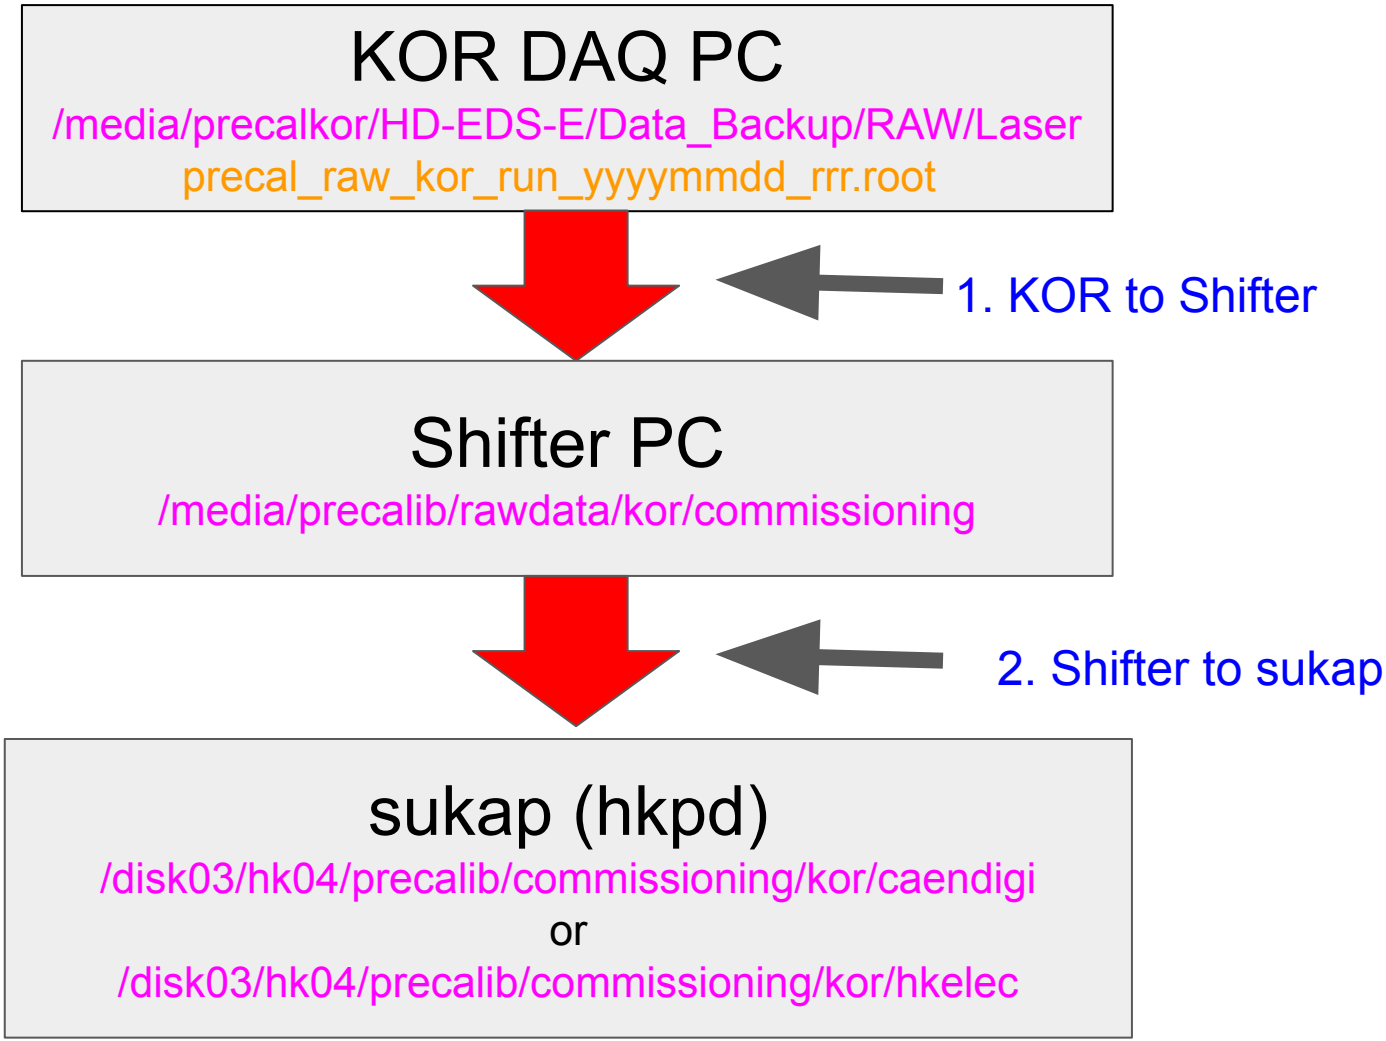
Data Copy System Manual for shifters KOR to Shifter Shifter to sukap


11 Oct 2026 Kotaro Kanai(UTokyo)
kanai@hep.phys.s.u-tokyo.ac.jp


Overview


KOR DAQ PC
/media/precalkor/HD-EDS-E/Data_Backup/RAW/Laser
precal_raw_kor_run_yyyymmdd_rrr.root
1. KOR to Shifter
Shifter PC
/media/precalib/rawdata/kor/commissioning
2. Shifter to sukap
sukap (hkpd)
/disk03/hk04/precalib/commissioning/kor/caendigi
or
/disk03/hk04/precalib/commissioning/kor/hkelec

1. KOR to Shifter on Shifter PC terminal

cd /home/precalib/shiftertool/copy
ls <- check the latest version (2026-10-11 : 0930-KORcopy,sh)
./0930-KORcopy.sh

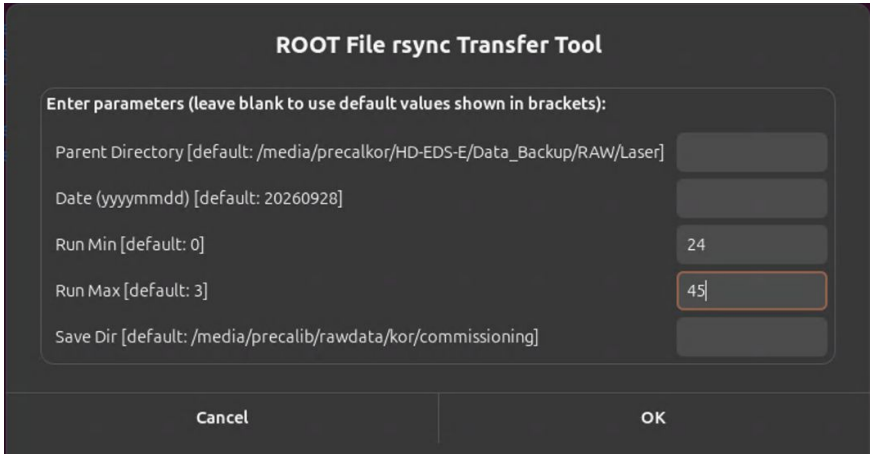


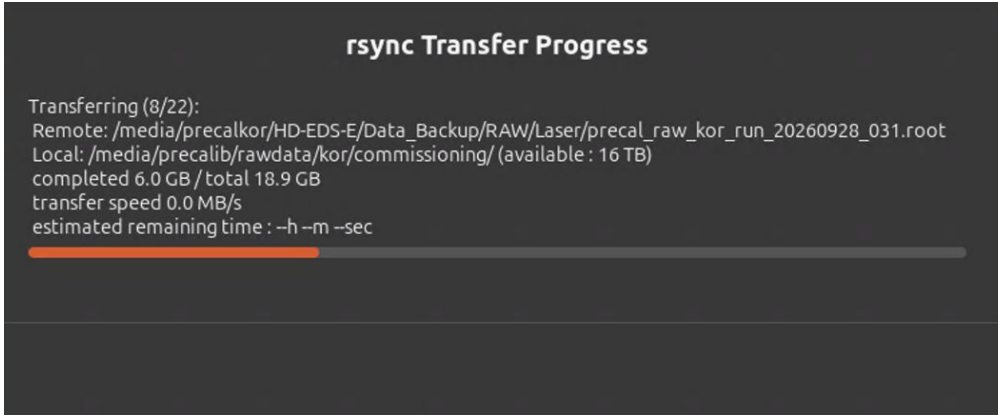

Progress window

input information
blank means default input
you may change Date and run numbers only

KOR to Shifter input window

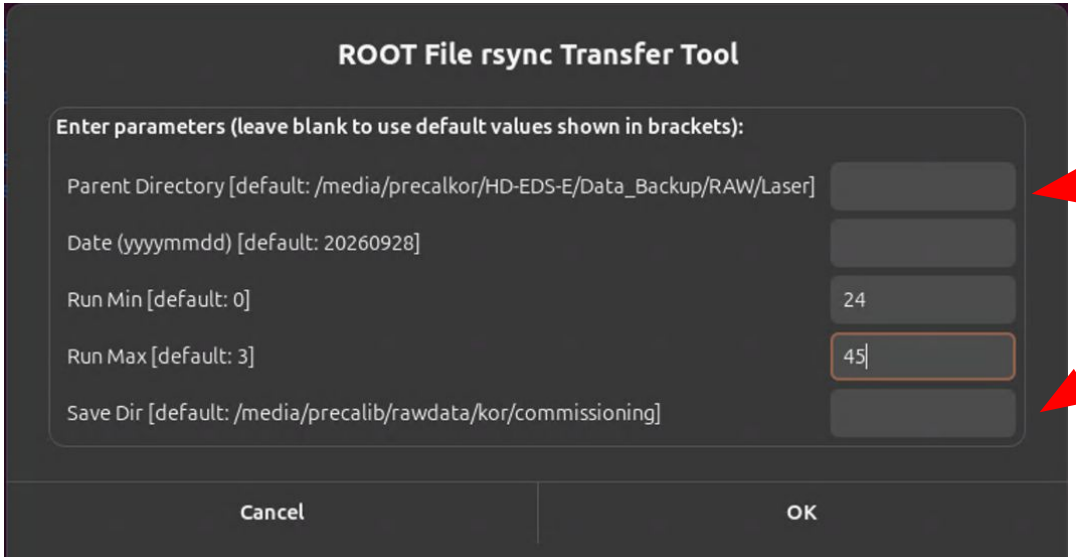


Leave them blank
No need to enter
folder names


NOTICE
Blank = default input

Parent directory : /media/precalkor/HD-EDS-E/Data_Backup/RAW/Laser
Date : yyyymmdd format
Run min and max : select run numbers over min, min+1,...max-1, max
Save Dir : /media/precalib/rawdata/kor/commissioning

2. Shifter to sukap(hkpd) on Shifter PC terminal

cd /home/precalib/shiftertool/copy
ls <- check the latest version (2026-10-11 : 0930-KORhkpd.sh)
./0930-KORhkpd.sh

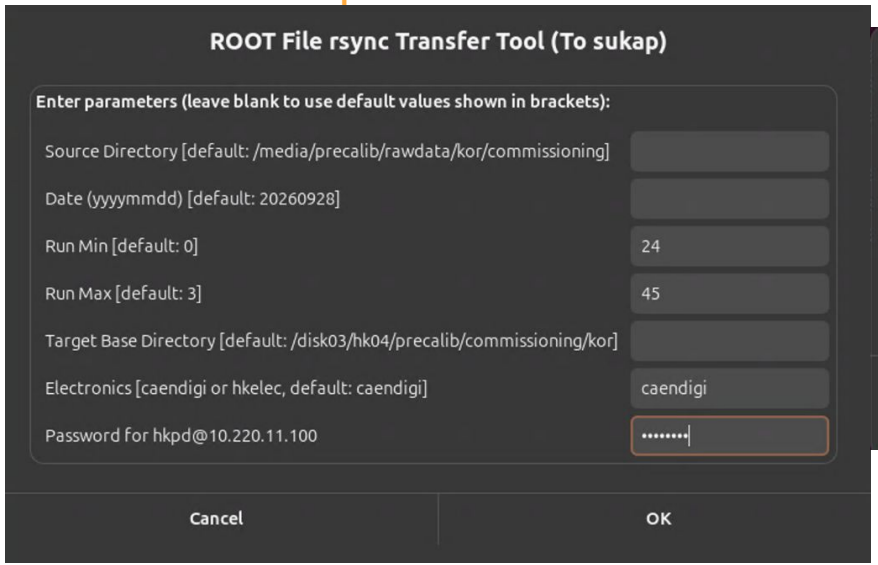


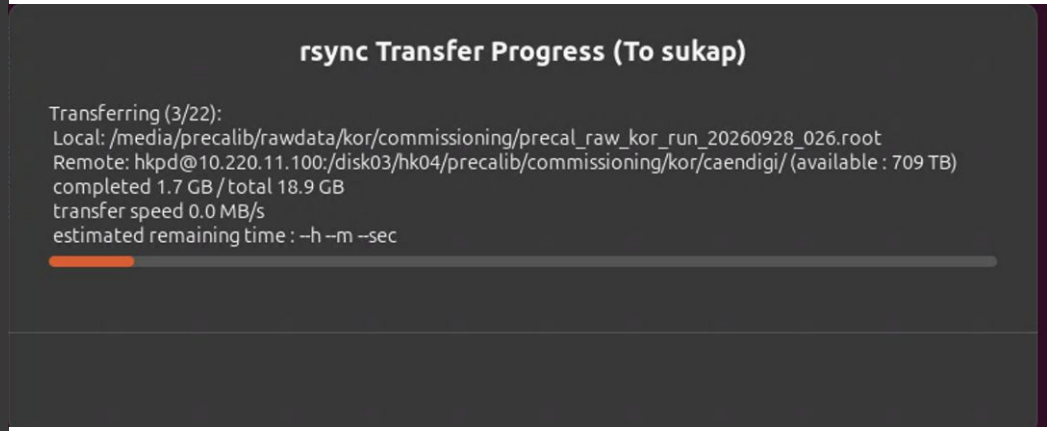

Progress window

input information
blank means default input
you may change Date and run numbers and electronics type(hkelec or canedigi)

Shifter to hkpd input window

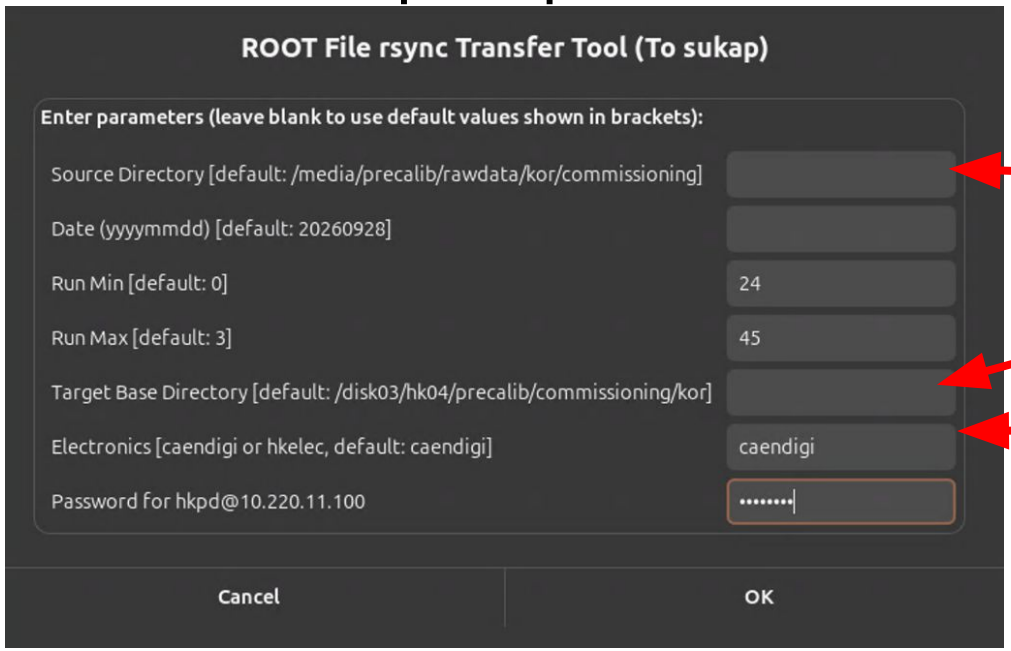


NOTICE
Blank = default input

Leave them blank
No need to enter
folder names


NOTICE
SELECT digitizer
type
caendigi or hkelec

Parent directory : /media/precalib/rawdata/kor/commissioning
Date : yyyymmdd format
Run min and max : select min max you want to transfer
Save Dir : /disk03/hk04/precalib/commissioning/kor
Electornics : caendigi or hkelec <-you must select the digitizer type

Shifter PC directory structure

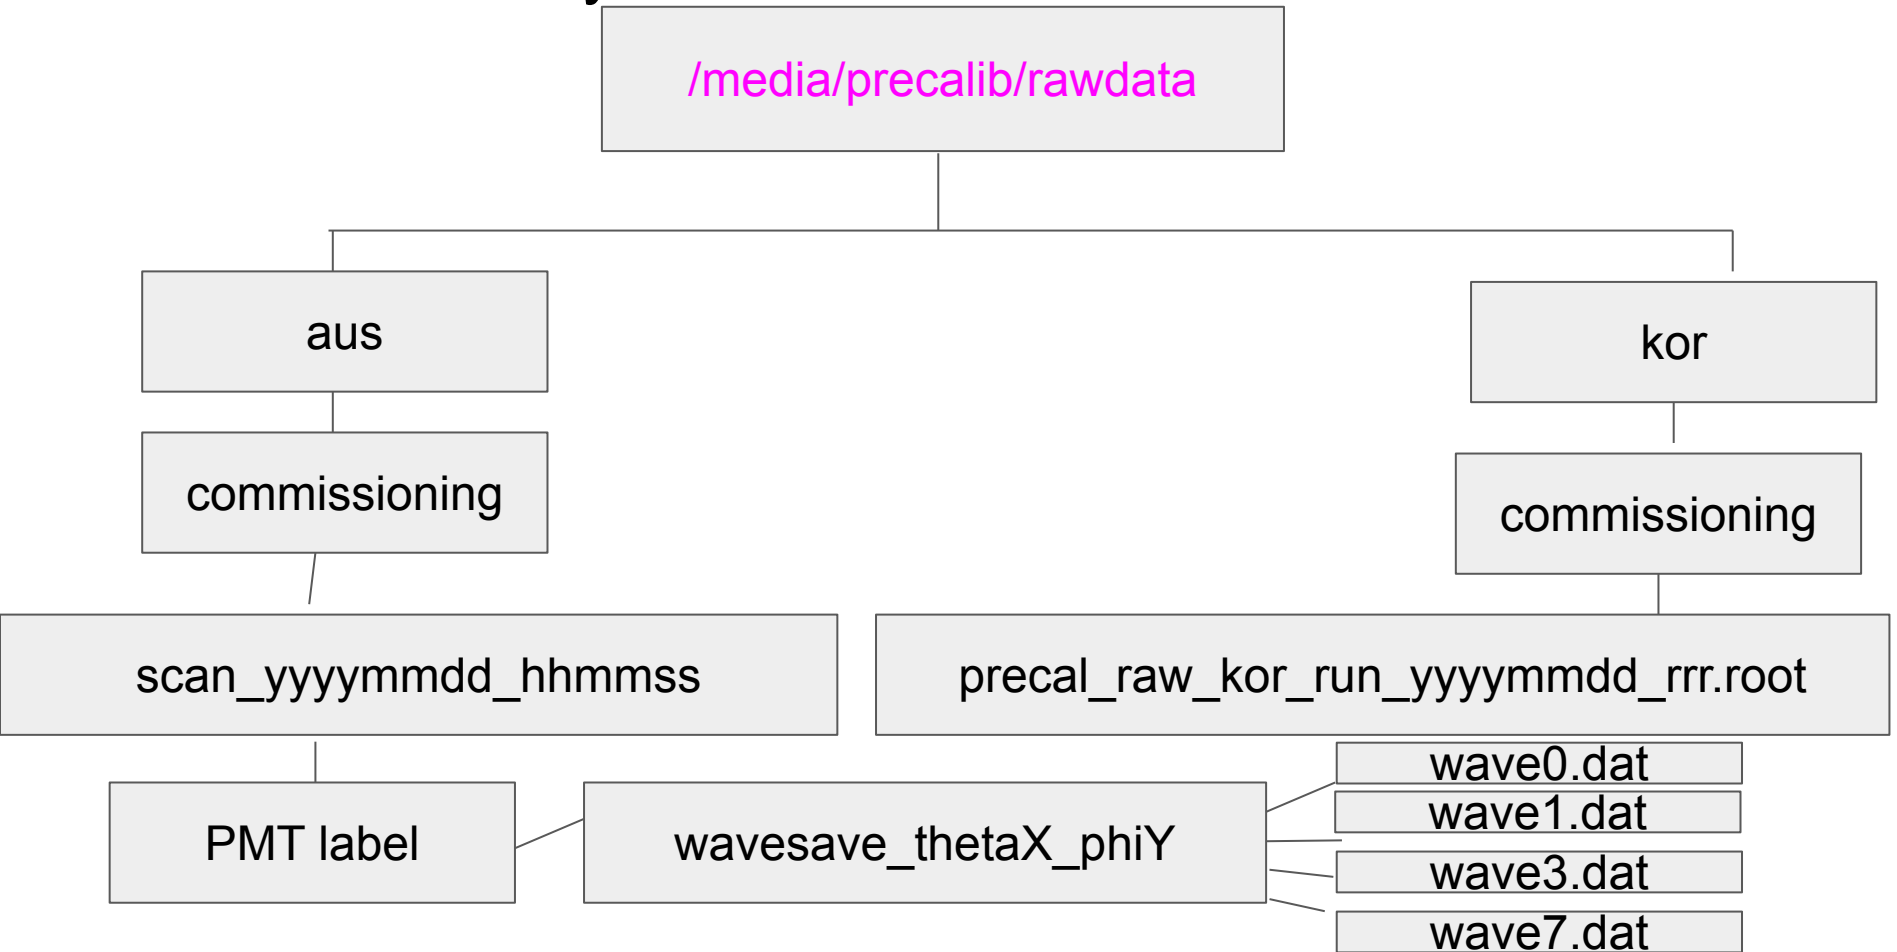


sukap(hkpd) directory structure

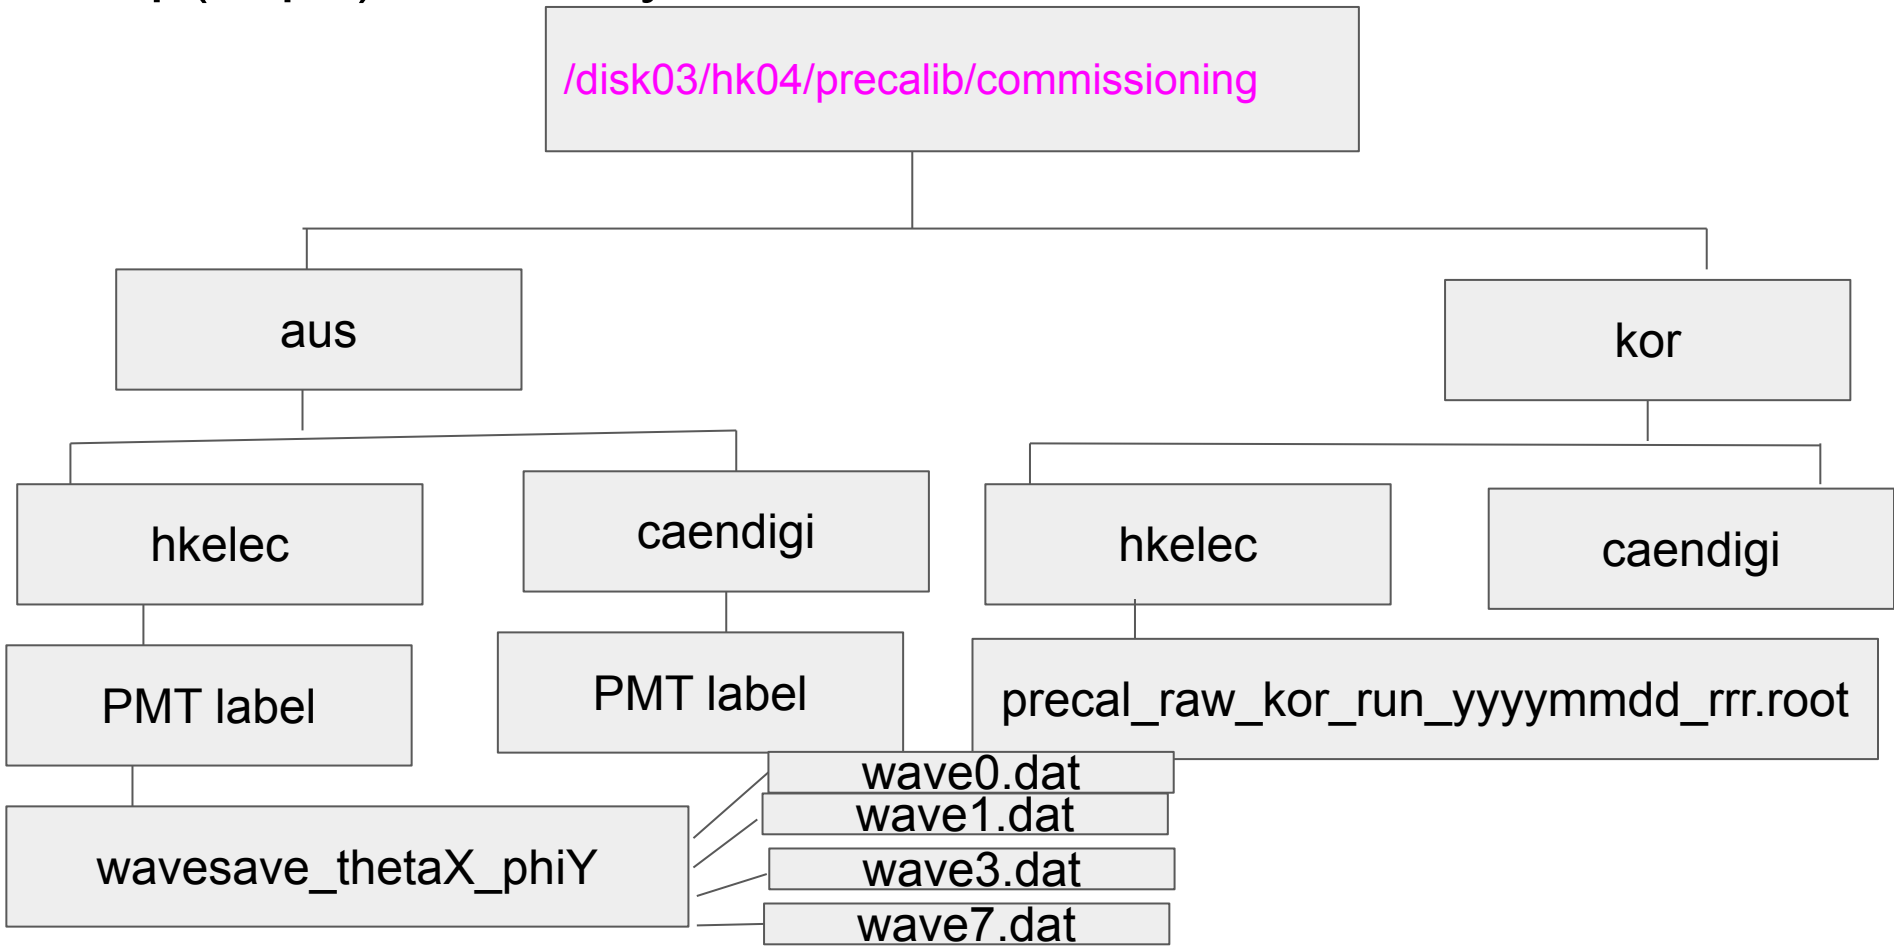

Parameter Information on Database

Shifters add all conditions they set to measure PMTs like this

date, name, time, PMT labels, HVs, B-current, wavelength, digitizer, LASER current etc

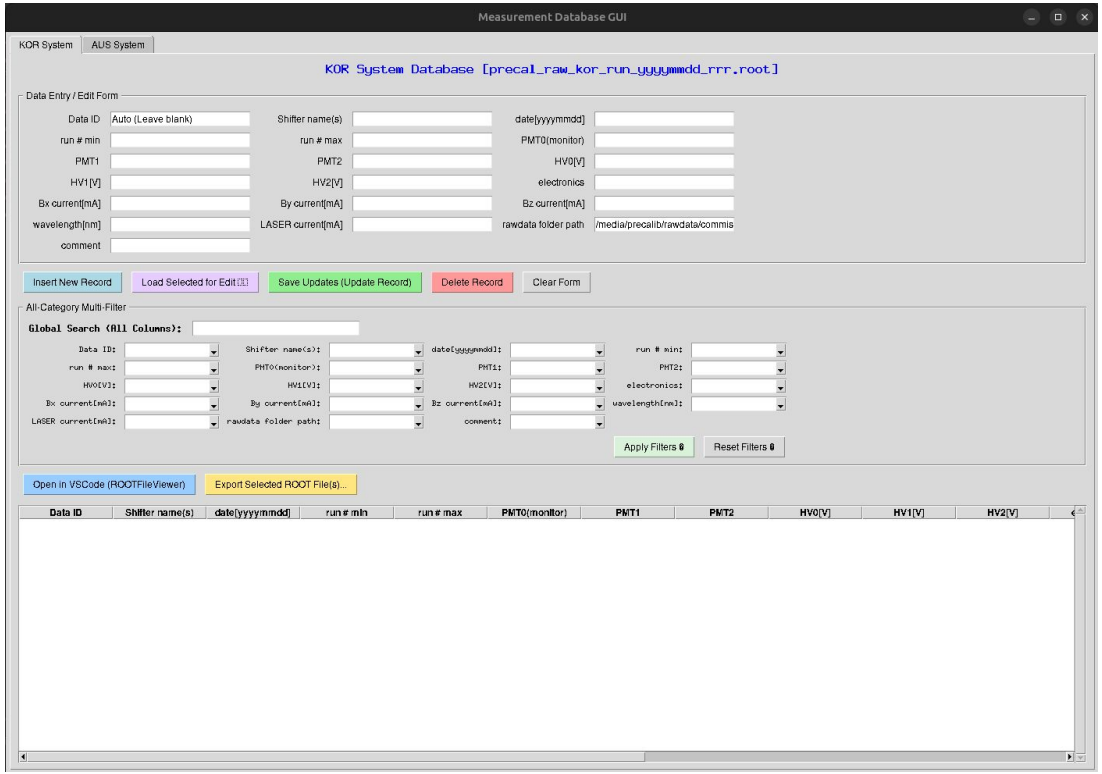

Appendix : PC information

・KOR DAQ : precalkor 192.168.0.104

ssh -v -p 4280 precalkor@192.168.0.104

Address: 1638953917

Password: precalkor1234!

ssh from Shifter PC

・Shifter PC : precalib 192.168.0.112

Anydesk : 1509405640

Pass ; hyperK1987A

・sukap : hkpd 10.220.11.100

ssh hkpd@10.220.11.100

hkpd password is unpublished

Ask Kanai, Ashida, Nakajima if you want

・B-field monitor

Anydesk : 1417899294

Pass : Kikusui18-5A