
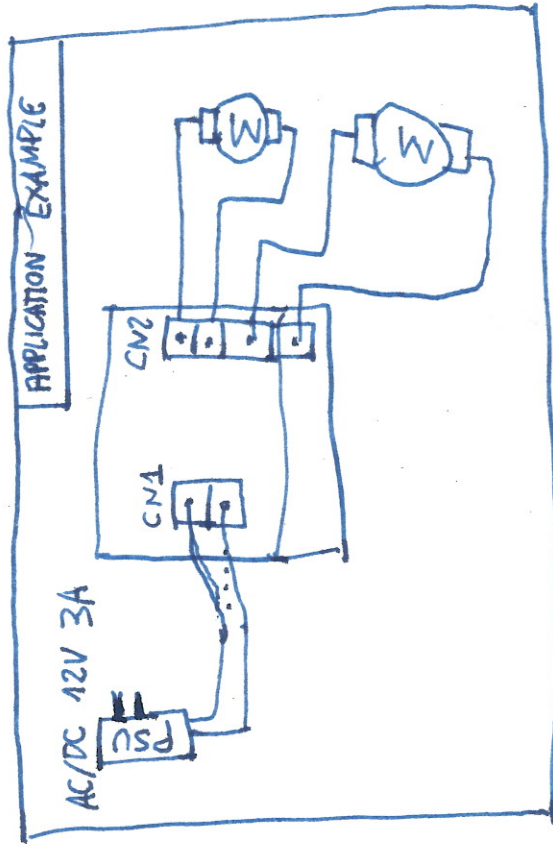



CIRCUIT DIAGRAM

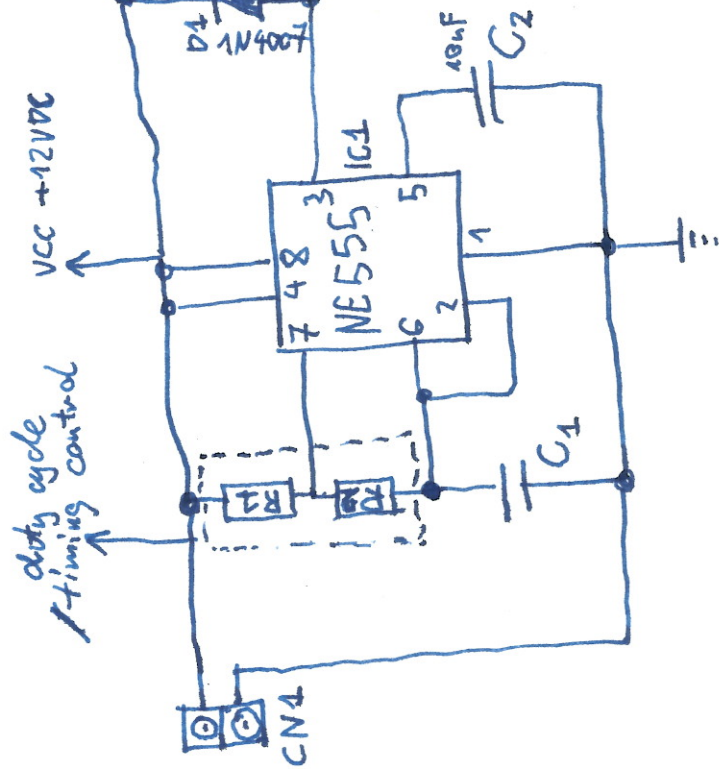

PARTS:
 C1: 222 CM1: ARKx2
 C2: 10nF CN2: ARKx4
 C3-C4:
 D1: 1N4007
 R1-R6: 222 RL1-RL2: 12V SPDT RELAY

ADJUSTMENTS: R1 R2 C1 → timing, duty cycle
 R3 R4 → inhaled pressure
 R5 R6 → exhaled pressure

USE VARIABLE
 RESISTORS
 OR RESISTOR
 LADDERS
 FOR R1-R6

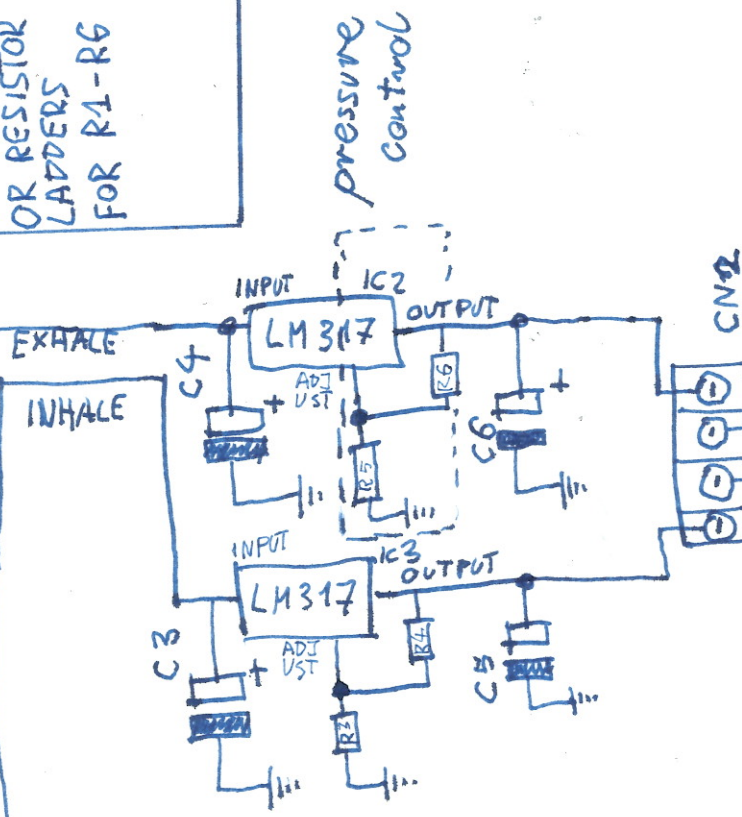

komrona
 IMPROVED
 CONTROLLER

AUTHOR	KACPER SOKOLOWSKI
LICENSE	CC BY
VENTILATOR	REV. 0.1.1.