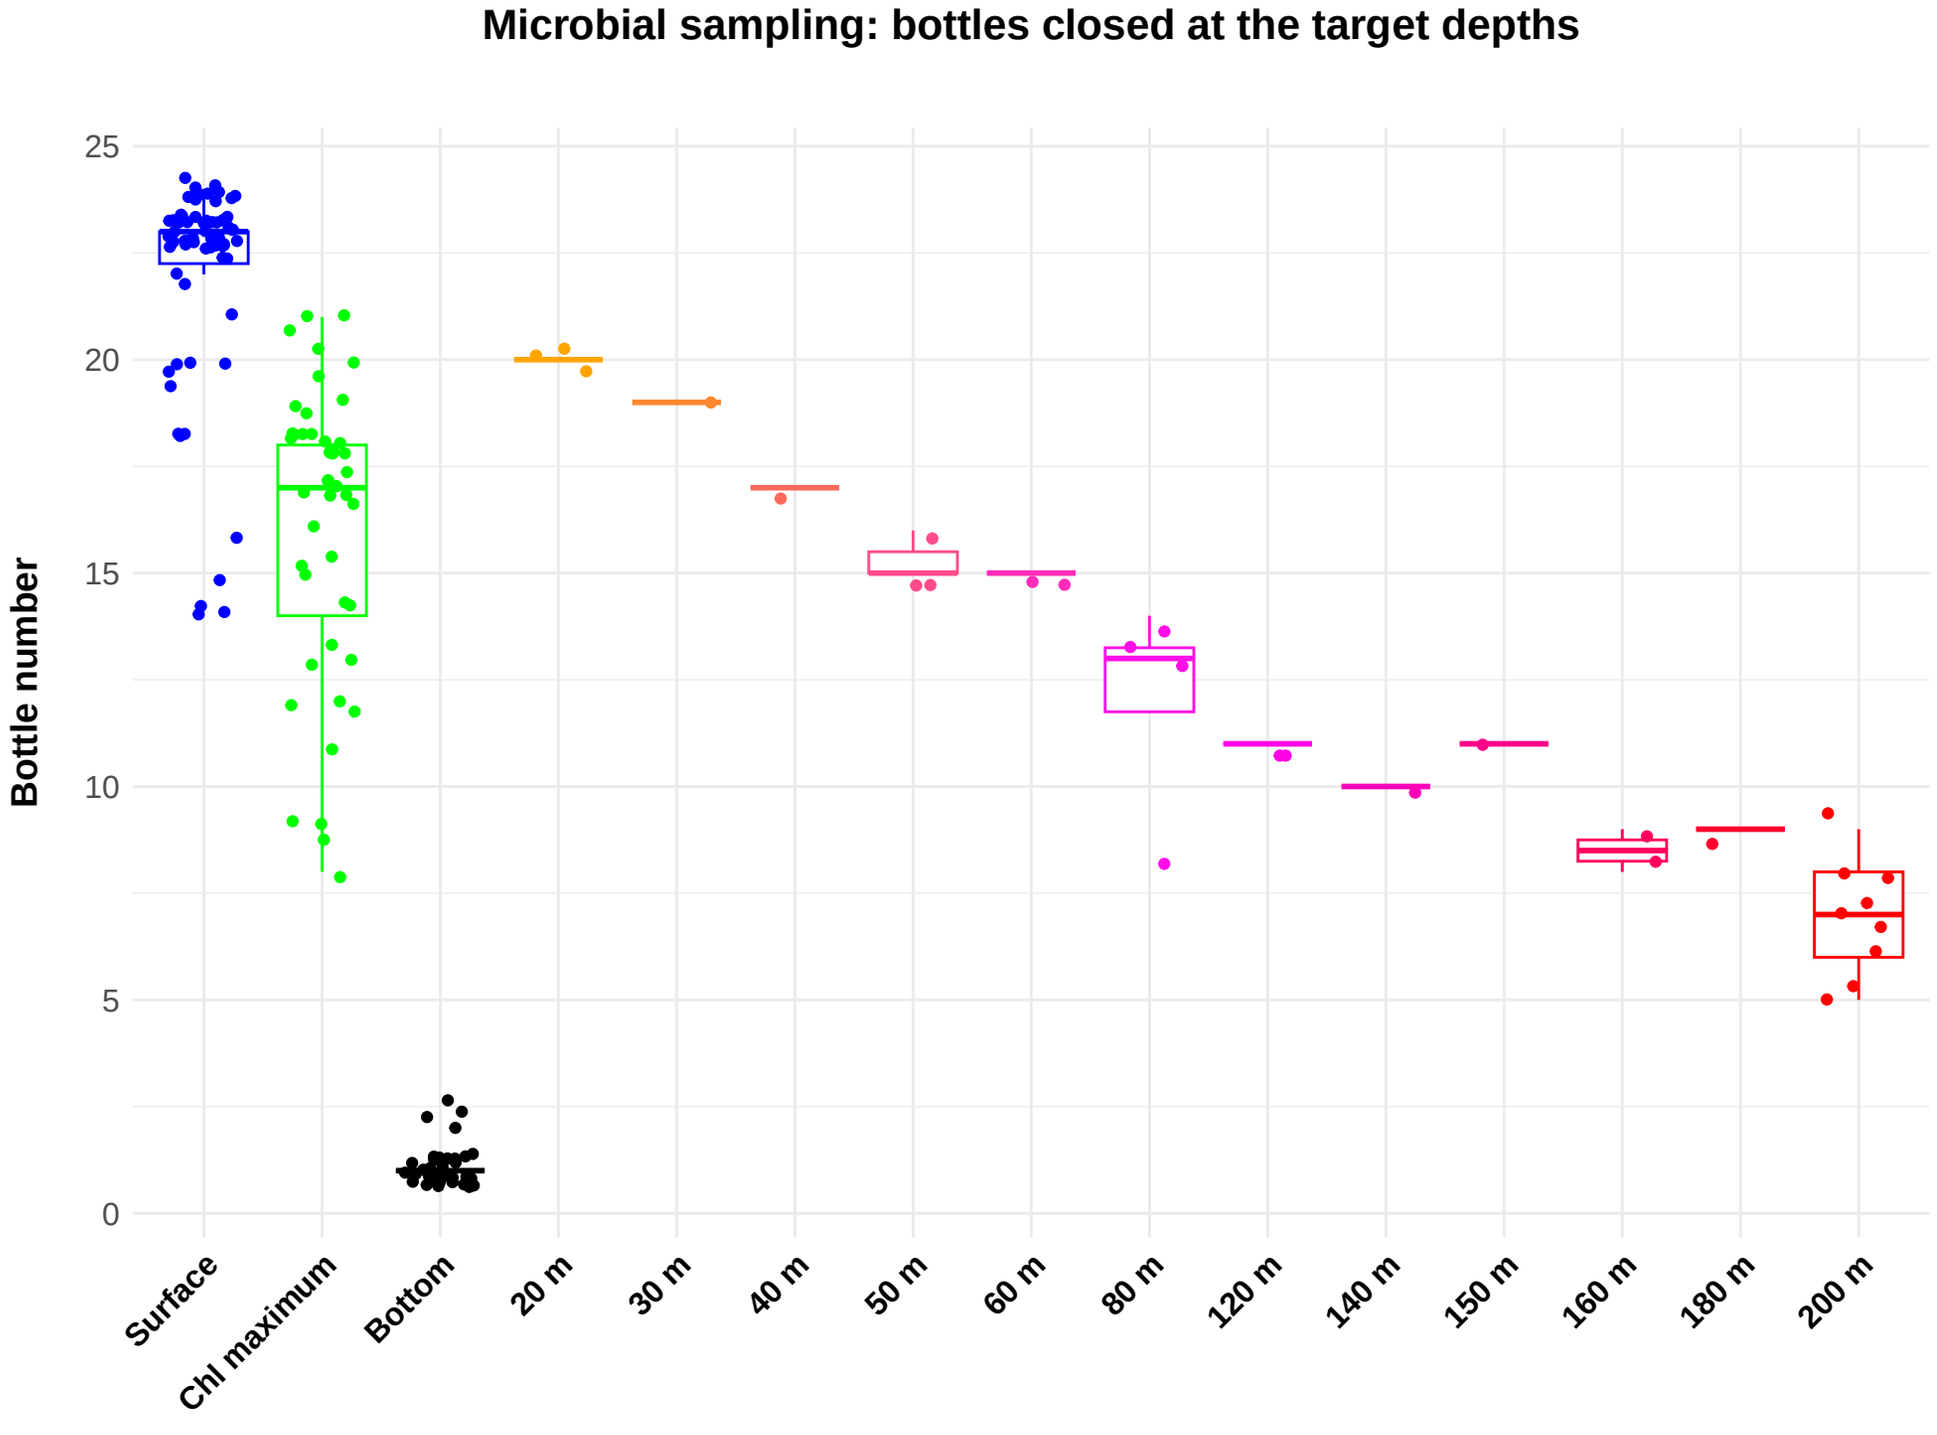
Microbial sampling: bottles closed at the target depths
Bottle number
25
20
15
10
5
0
Surface
Chl maximum
Bottom
20 m
30 m
40 m
50 m
60 m
80 m
120 m
140 m
150 m
160 m
180 m
200 m

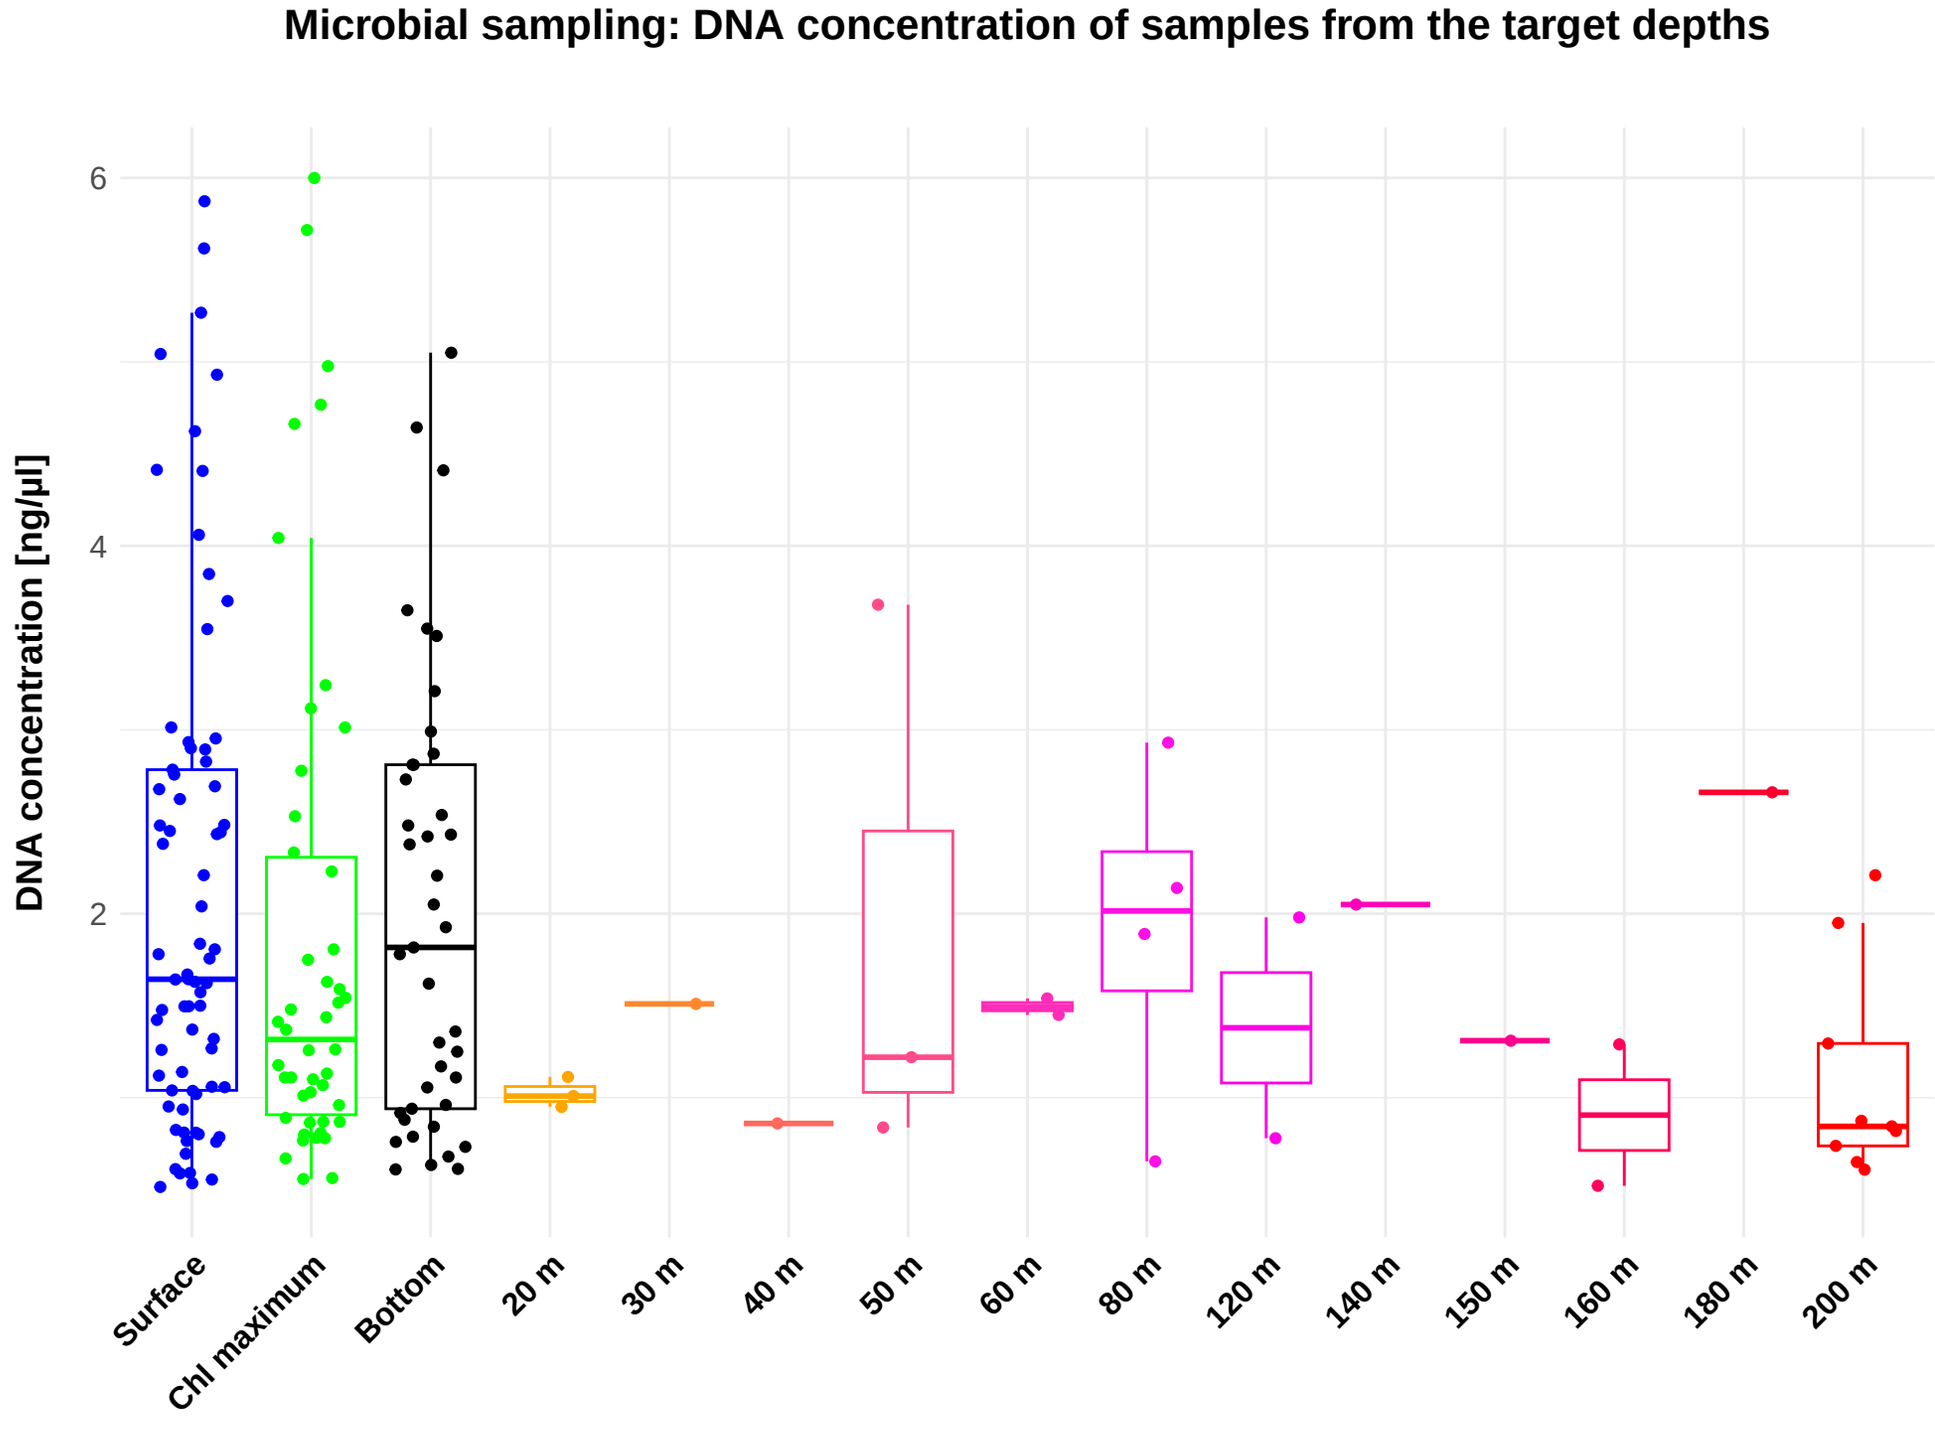
Microbial sampling: DNA concentration of samples from the target depths
DNA concentration [ng/µl]
6
4
2
Surface
Chl maximum
Bottom
20 m
30 m
40 m
50 m
60 m
80 m
120 m
140 m
150 m
160 m
180 m
200 m