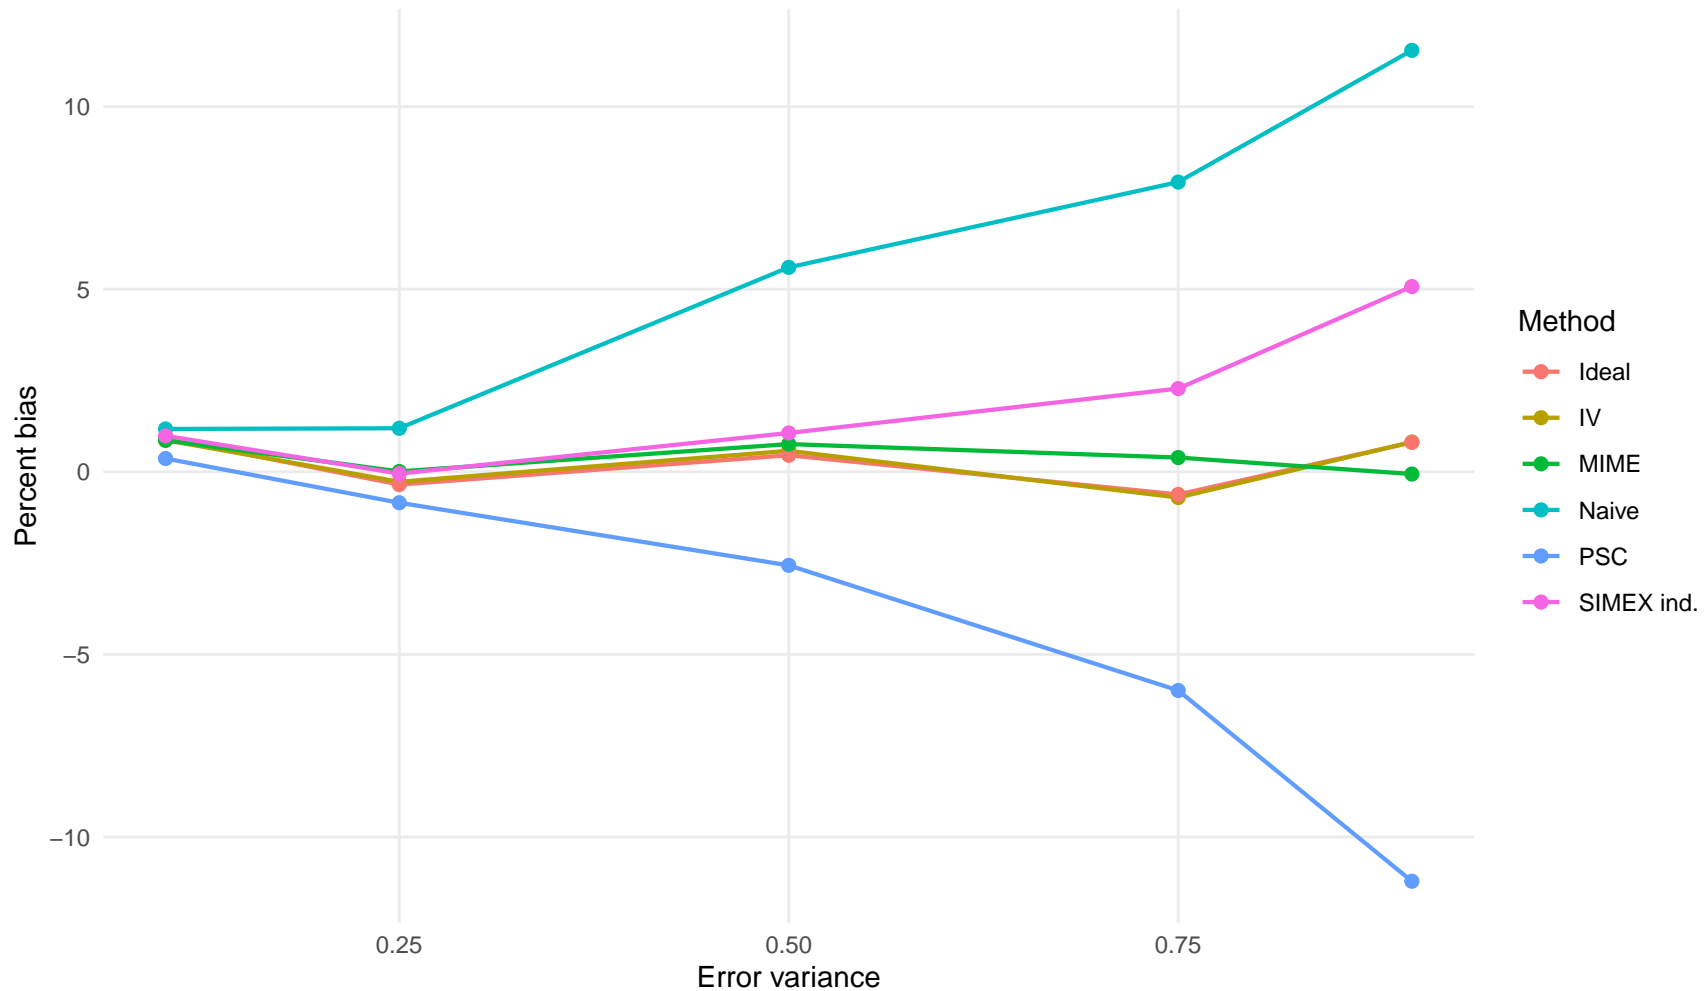**Percent bias of ME correction methods**

Varying Error variance

True ATE: 1, Sample size: 1500, Binary outcome: 0, Corr(X,Z): 0.25, Corr(X,V): 0.5, ax: 0.25