
Test Spectrum

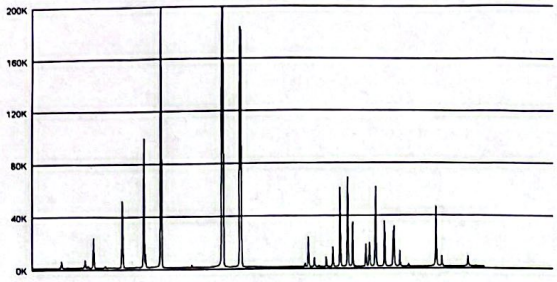

Ocean Insight

Wavelength Calibration Data Sheet

Built for:
Order Number: **1342218**
Model: **QEPRO-ABS**
Grating: GRATING_#HC1 - 300 Line Composite Blaze
Bandwidth: 201 - 989 nm
Options: DET-QE-OFLV-200 Detector, NoneLens, INTSMA-010 Slit,
Serial Number: **QEP05181**

λ	Pixel #	Predicted λ	Δλ
253.652	70	253.544	0.108
296.728	125	296.693	0.035
334.148	172	334.189	-0.041
340.365	180	340.374	-0.009
365.015	212	365.129	-0.114
404.656	262	404.554	0.102
435.834	302	435.752	0.082
546.074	445	546.042	0.032
576.959	485	576.991	-0.032
585.249	496	585.243	0.006
594.483	508	594.479	0.004
597.553	512	597.537	0.016
602.999	519	602.998	0.001
614.306	534	614.327	-0.021
621.728	544	621.720	0.008
626.649	550	626.665	-0.016
633.443	559	633.462	-0.019
636.235	563	636.245	-0.010
643.847	573	643.861	-0.014
667.828	604	667.820	0.008
671.704	609	671.694	0.010
696.543	642	696.519	0.024
738.398	698	738.413	-0.015
743.890	705	743.877	0.013
748.887	712	748.895	-0.008
763.511	732	763.559	-0.048
785.482	761	785.482	0.000
794.818	774	794.871	-0.053
811.531	796	811.305	0.226
826.324	816	826.316	0.008
826.452	816	826.419	0.033
828.012	819	828.009	0.003
829.811	821	829.833	-0.022
834.682	828	834.698	-0.016
842.465	838	842.339	0.126
852.144	851	852.116	0.028
912.297	933	912.271	0.026
922.450	947	922.434	0.016

This is a sample of calibration peaks used as there were more than can be shown on this page

Calibration Coefficients

First Coefficient:	0.7997204661
Second Coefficient:	-3.36941e-005
Third Coefficient:	-2.73891e-009
Intercept:	197.45384216
Regression Fit:	0.9999998808

Stray Light Measurements (AU)

Holmium Oxide (444nm):	1.66
Yellow Dye:	2.42
Blue Dye:	2.72
Molybdate:	1.78
OG550 Filter:	2.78
RG850 Filter:	2.86
FG3 Filter:	1.26

Calibrated By: carlos.irizarry
Calibrated: 22-August-2022

Scanned with CamScanner