



Measurements that pass QC


head length

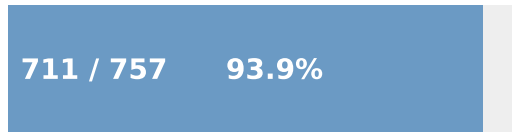

head width

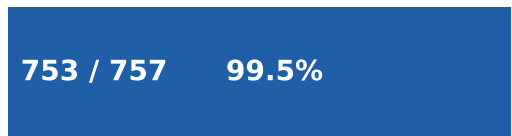

The HL failure is structured, not random
29 of 46 genera (n≥5) have zero inversions

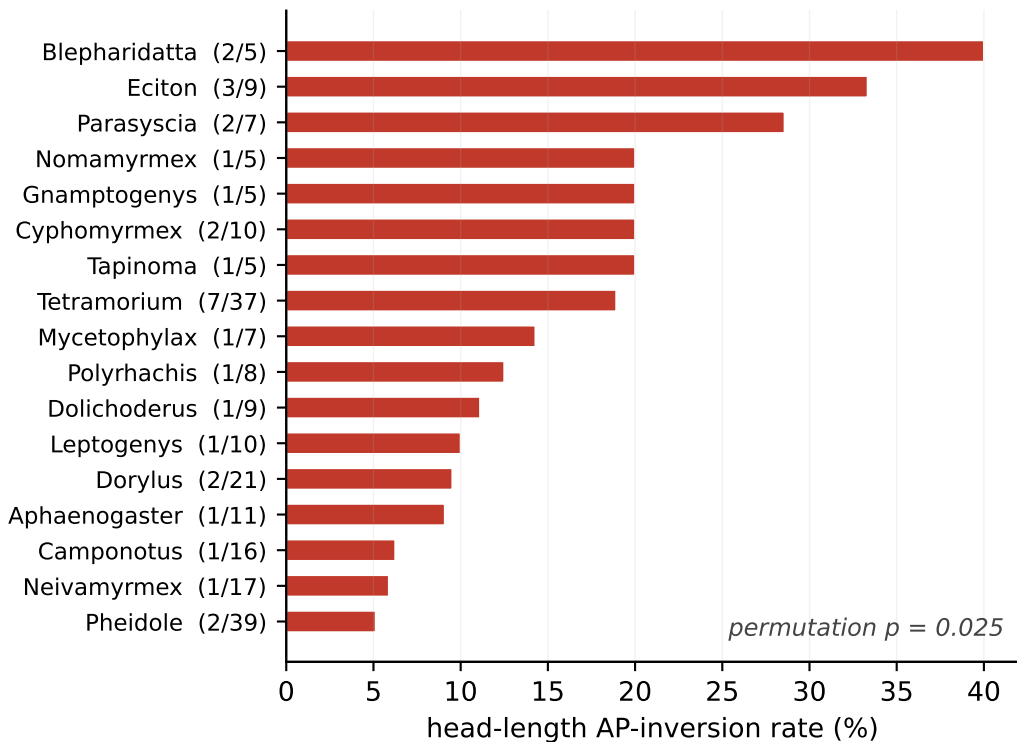

0 200 400 600
specimens admissible (of 757 fitted)