

01 Executive summary

Revenue grew across all three regions. Retention improved in the West, while the South remains below the 95 percent target.


Quarterly business review · Q1–Q4 · three regions · revenue and retention.

02 Regional evidence

REGION	REVENUE	RETENTION	STATUS
North	184	94.1%	Watch
South	156	92.8%	Below target
West	211	95.0%	On plan

03 Analysis

Quarterly retention

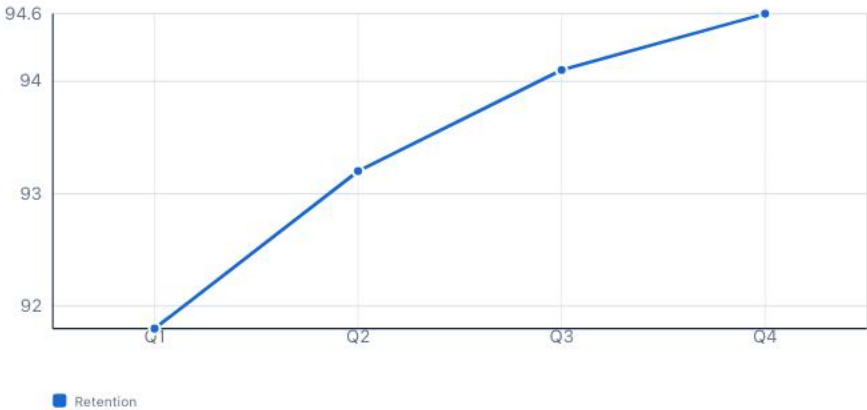

Line Chart: 4 rows · X Quarter · Y Retention · 2 fields

04 Decision



Proceed with monitored revenue recovery
Close the South retention gap before the next review.

Review

05 Decision and next step



Next step: close the South retention gap before the next quarterly review.

06 Performance

Regional revenue

551

Delta —

Retention

94.6%

Current performance

Delta 2.8

Quarterly retention

Before

91.8 %

After


94.6 %



Target 95%

Affected lot L2407 shows a localized die-level yield loss after ETCH-08 chamber A processing. Contain the lot until the chamber check and paired reference run confirm recovery.

Lot L2407 · ETCH-08 chamber A · affected die compared with a paired reference · release held for verification.





EVIDENCE	AFFECTED	REFERENCE	INTERPRETATION
Yield distribution	94.2%	98.6%	Mean of observed cohorts
Affected lot L2407	94.2%	—	Localized die loss
ETCH-08 / A	Pressure +2.1%	Stable	Verify chamber


Contain lot L2407 through chamber requalification

Contain

Release only after chamber A and the paired reference run confirm recovery.

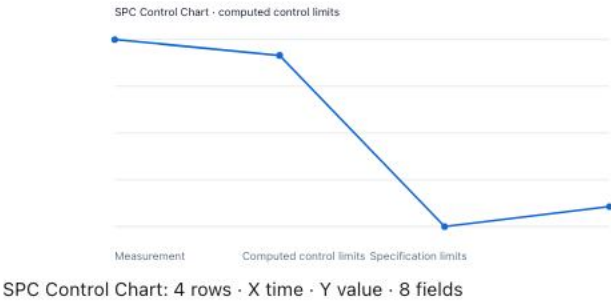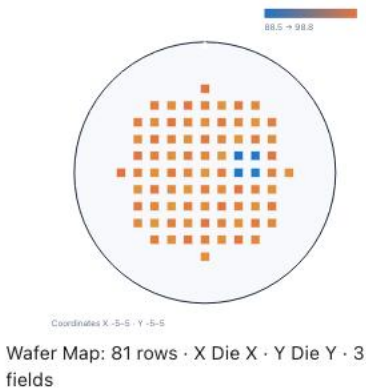

Control versus affected distribution

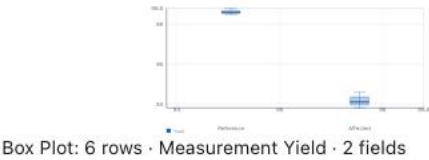

Verified finding

	Finding · chamber A pressure drift aligns with the L2407 yield excursion.
Affected yield is 94.2% versus 98.6% reference. Contain L2407 and verify the matched chamber run before release.	
Evidence	Verified

Affected versus reference yield



Affected yield

94.2%

Delta -4.4

Target 95%


01 Experiment summary

The treatment cohort improved conversion across four weeks. The quality guardrail remained inside its agreed range; the sample does not establish long-term retention.

Eligible new-account cohorts · W1–W4 · randomized control and treatment · conversion and quality guardrail.

02 Analysis

Conversion by week

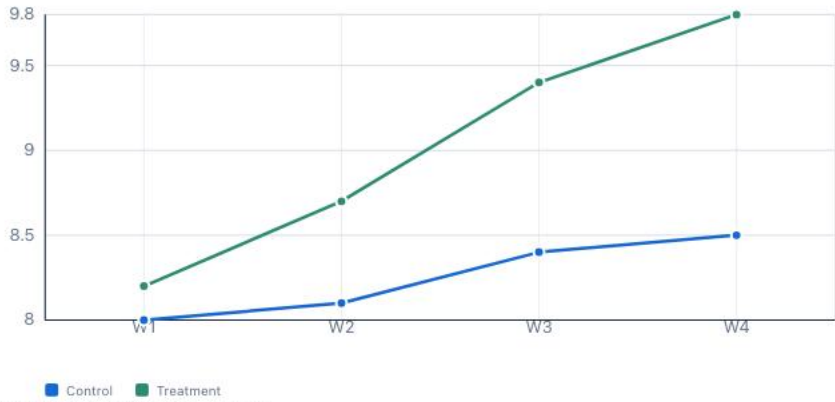

Treatment conversion rose from 8.2% in week 1 to 9.8% in week 4; the control moved from 8.0% to 8.5%. The treatment distribution is higher across this sample, with all three cohort checks inside the quality guardrail. Continue only as a limited rollout because these four weeks do not establish long-term retention.

Outcome distribution by cohort



03 Experiment evidence

Cohort evidence

COHORT	ELIGIBLE	CONVERSION	QUALITY GUARDRAIL
Control	1198	8.25%	Within quality guardrail
Treatment	1204	9.03%	Within quality guardrail
Holdout	412	8.45%	Monitor mix

04 Recommendation




Stage a limited treatment rollout

Pause expansion if the quality guardrail moves outside its agreed range.

Review

05 Performance

Treatment conversion · Week 1 to 4

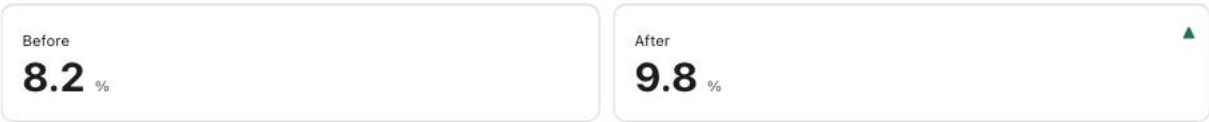

Treatment conversion

9.8%

Delta 1.6

Target 10%


01 Operating summary

Shift B recovered yield after chamber maintenance. Keep the recipe locked through the next paired-lot check and hand off the evidence to Quality and Equipment Engineering.

Line 4 · shifts A–C · chamber A controls · capacity release review.

02 Analysis

Yield by shift

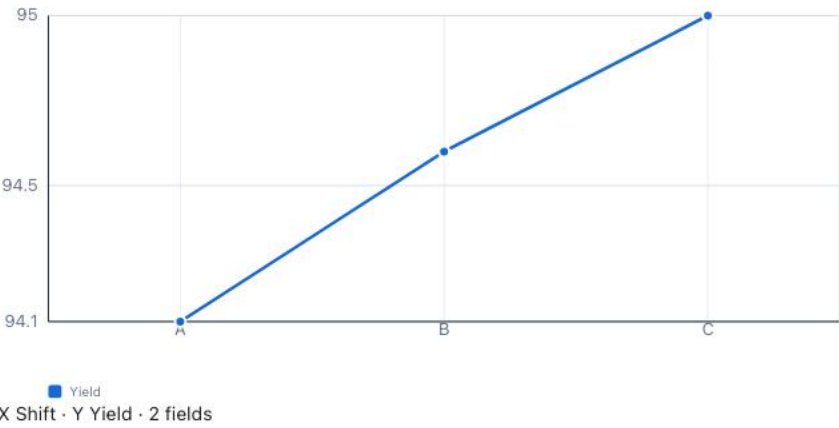

Line Chart: 3 rows · X Shift · Y Yield · 2 fields

SPC Control Chart · computed control limits · specifications shown



SPC Control Chart: 5 rows · X Time · Y Measurement · 4 fields

Yield recovered from 94.1% on shift A to 95.0% on shift C, while the control sample remains within specification. Keep the recipe locked until the next paired-lot check closes the two open items.

03 Response workflow



TOOL	CHAMBER	MEASURE	OWNER	STATUS
ETCH-08	A	Pressure	Equipment Eng.	Open
ETCH-07	C	Flow	Process Eng.	Stable
MET-02	B	Yield	Quality	Verified



Measurement system remains within the qualified reference range.

Sample: 30 parts · method: inline metrology · source: shift B inspection.

Evidence

Verified

04 Decision



Hold added capacity until the paired-lot check closes
Keep the recipe locked and attach the next-shift control evidence.

Review

05 Next steps

Complete chamber verification and update the runbook.

Active

Owner: Equipment Engineering · due next shift · evidence: paired control lot.

06 Performance

First pass yield

95%

Delta 0.9

Unplanned downtime

8.3h

Target 96%

Delta -1.7

Target 6 h

Order volume rose while returns fell across the spring launch.

Monthly operating review · Jan–Apr · Source: order and returns ledger.

April orders

1611

Delta 331

vs prior period

Order growth since January

331 orders

Delta —

vs prior period

Monthly returns

Before


42

After

31



Orders by month

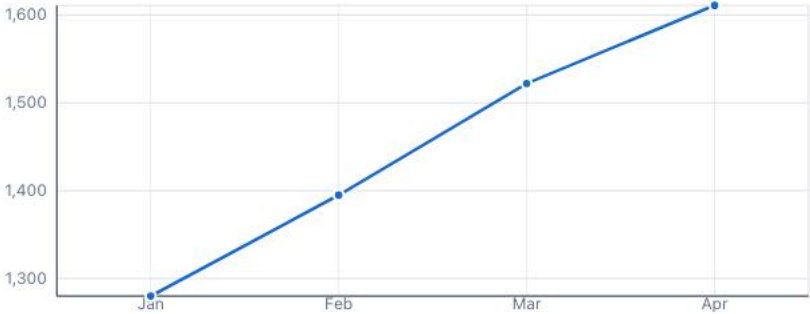

Orders

Line Chart: 4 rows · X Month · Y Orders · 3 fields

Returns by month



Value

Line Chart: 4 rows · X Month · Y Returns · 3 fields

Order volume increased through the spring launch. Returns declined each month; continue weekly review while the fulfillment mix changes.

Review path



Order and return evidence

MONTH	ORDERS	RETURNS
Jan	1280	42
Feb	1395	38
Mar	1522	35
Apr	1611	31
Change	331	–11



Review rising orders alongside falling returns

Check the fulfillment mix before changing the spring capacity plan.

Review



Next step: review the return mix before changing fulfillment capacity.

01 Situation

Keep Bridge C-08 closed until Span 4 crack gauge data is verified.

Overnight load testing cleared two required checks. The Span 4 crack gauge export has not synchronized; water level is still receding, so the reopening decision remains pending.

02 Disposition

Reopening gate



Do not reopen Bridge C-08 yet.

The required Span 4 crack-gauge result is unavailable. Passing load checks at the approach joint and Pier 2 do not establish Span 4 clearance.

HOLD - one required result missing



Next step: synchronize the Span 4 gauge file, verify the crack trend, and repeat disposition before the 06:00 maintenance handover.

03 Inspection evidence

Overnight inspection record

LOCATION	OBSERVED LOAD	REQUIRED	DISPOSITION
Approach slab joint	1.34x	≥ 1.25x	Pass
Pier 2 bearing	1.29x	≥ 1.25x	Pass
Span 4 crack gauge	Not synced	Verified reading	Open

Verified load checks

2/3 required

Delta 1 pending - Span 4

Target 3 / 3 required