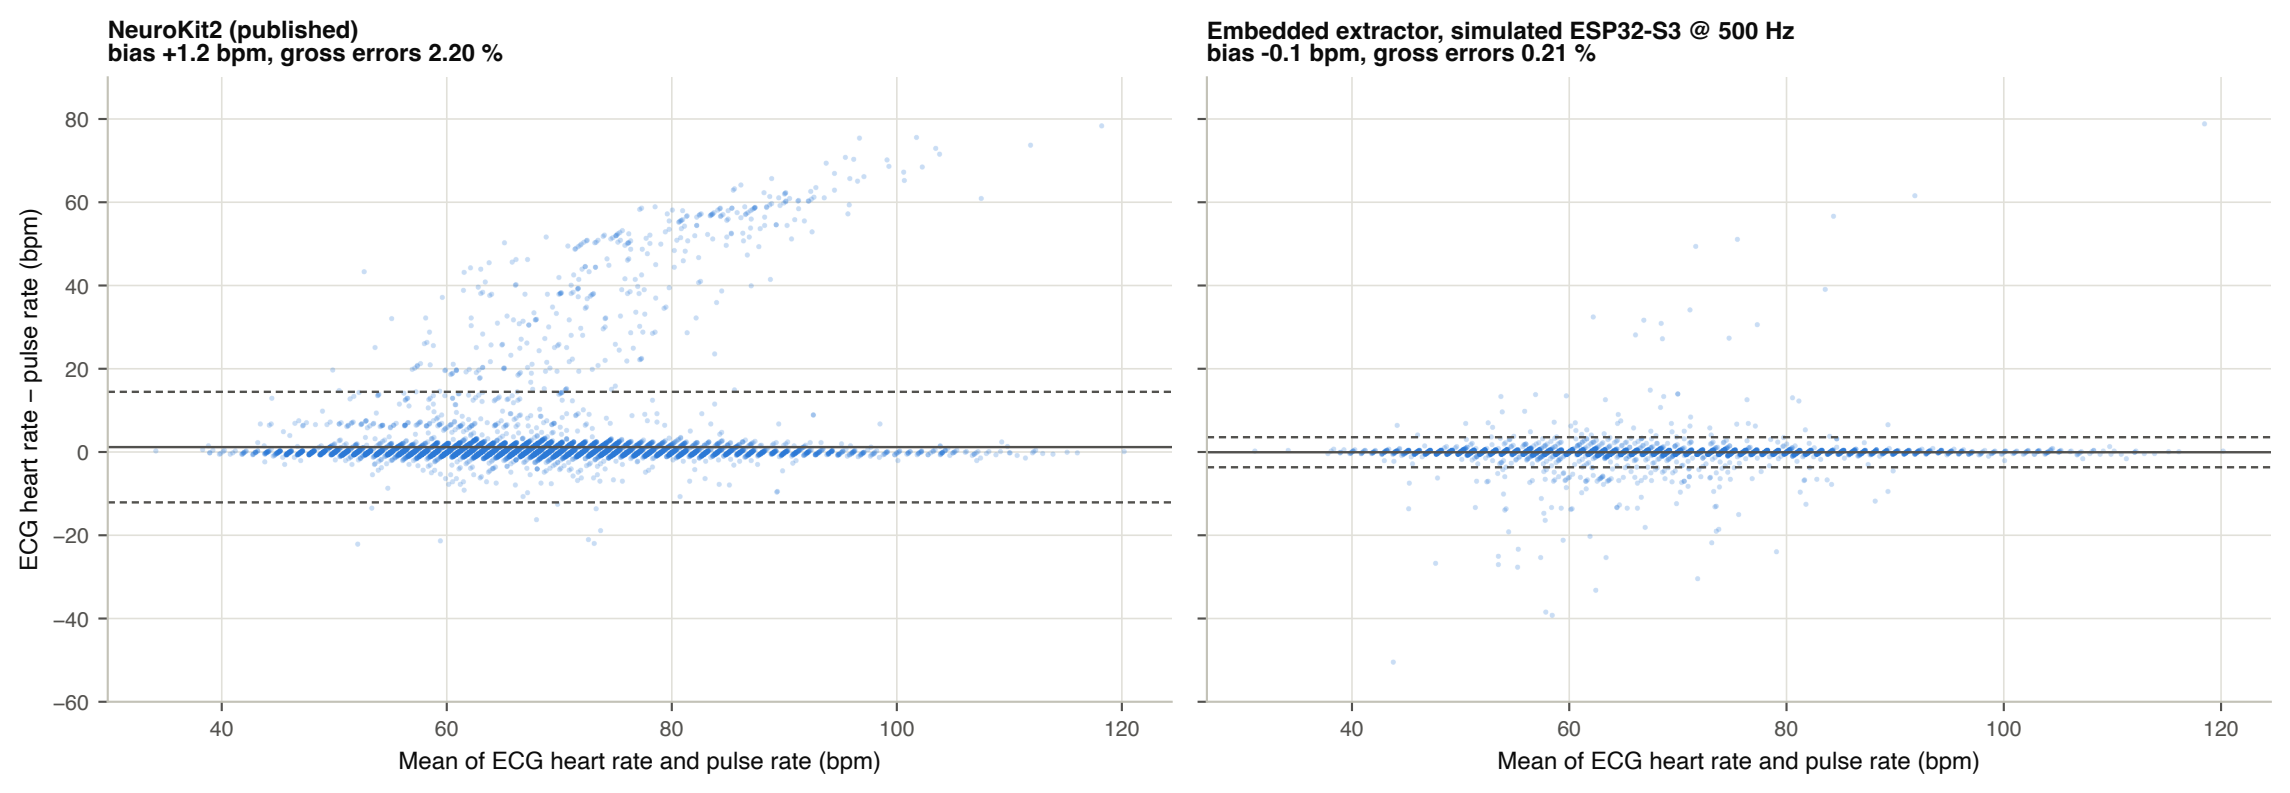

NeuroKit2 (published)
bias +1.2 bpm, gross errors 2.20 %
Embedded extractor, simulated ESP32-S3 @ 500 Hz
bias -0.1 bpm, gross errors 0.21 %
ECG heart rate − pulse rate (bpm)
80
60
40
20
0
−20
−40
−60
40
60
80
100
120
Mean of ECG heart rate and pulse rate (bpm)
Mean of ECG heart rate and pulse rate (bpm)