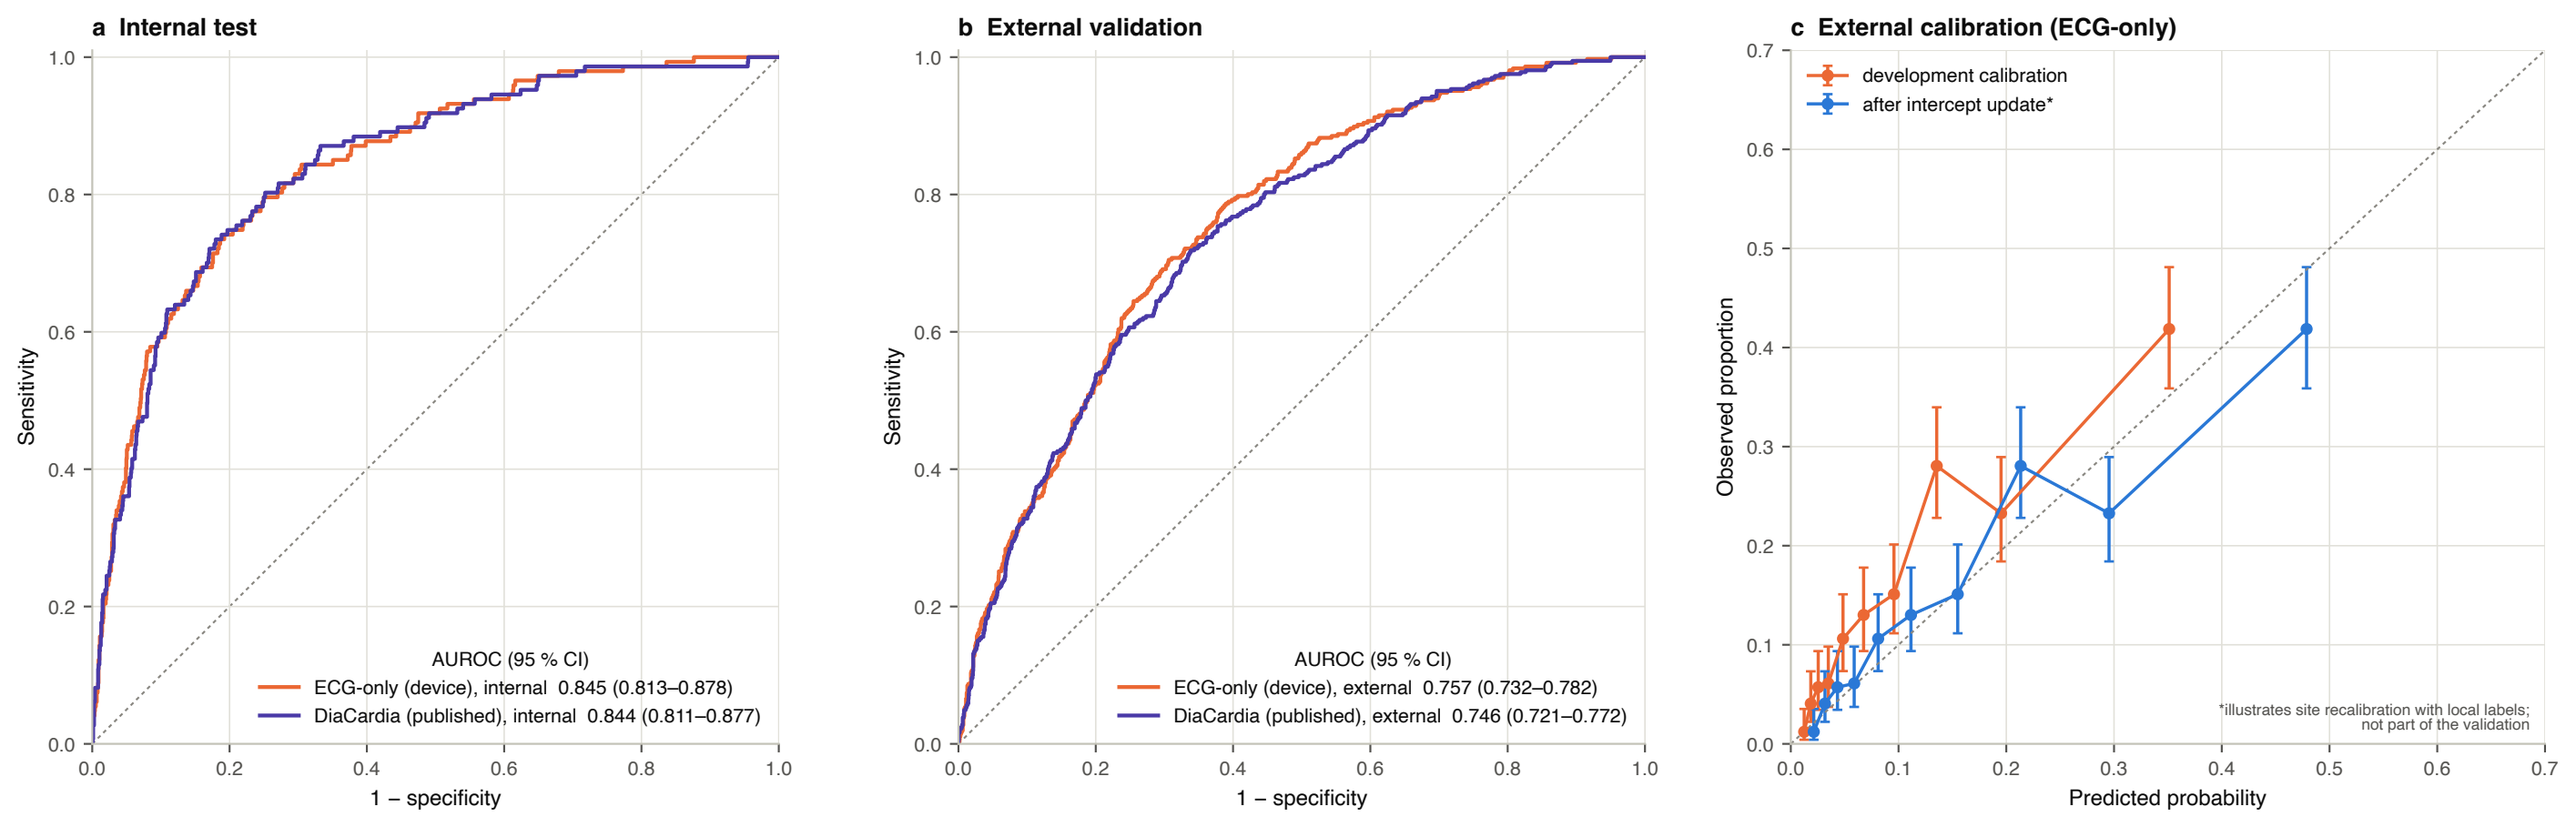
a Internal test
Sensitivity
1 – specificity
AUROC (95 % CI)
ECG-only (device), internal 0.845 (0.813–0.878)
DiaCardia (published), internal 0.844 (0.811–0.877)
b External validation
Sensitivity
1 – specificity
AUROC (95 % CI)
ECG-only (device), external 0.757 (0.732–0.782)
DiaCardia (published), external 0.746 (0.721–0.772)
c External calibration (ECG-only)
development calibration
after intercept update*
Observed proportion
Predicted probability
*illustrates site recalibration with local labels;
not part of the validation