


HEALTH SYSTEMS

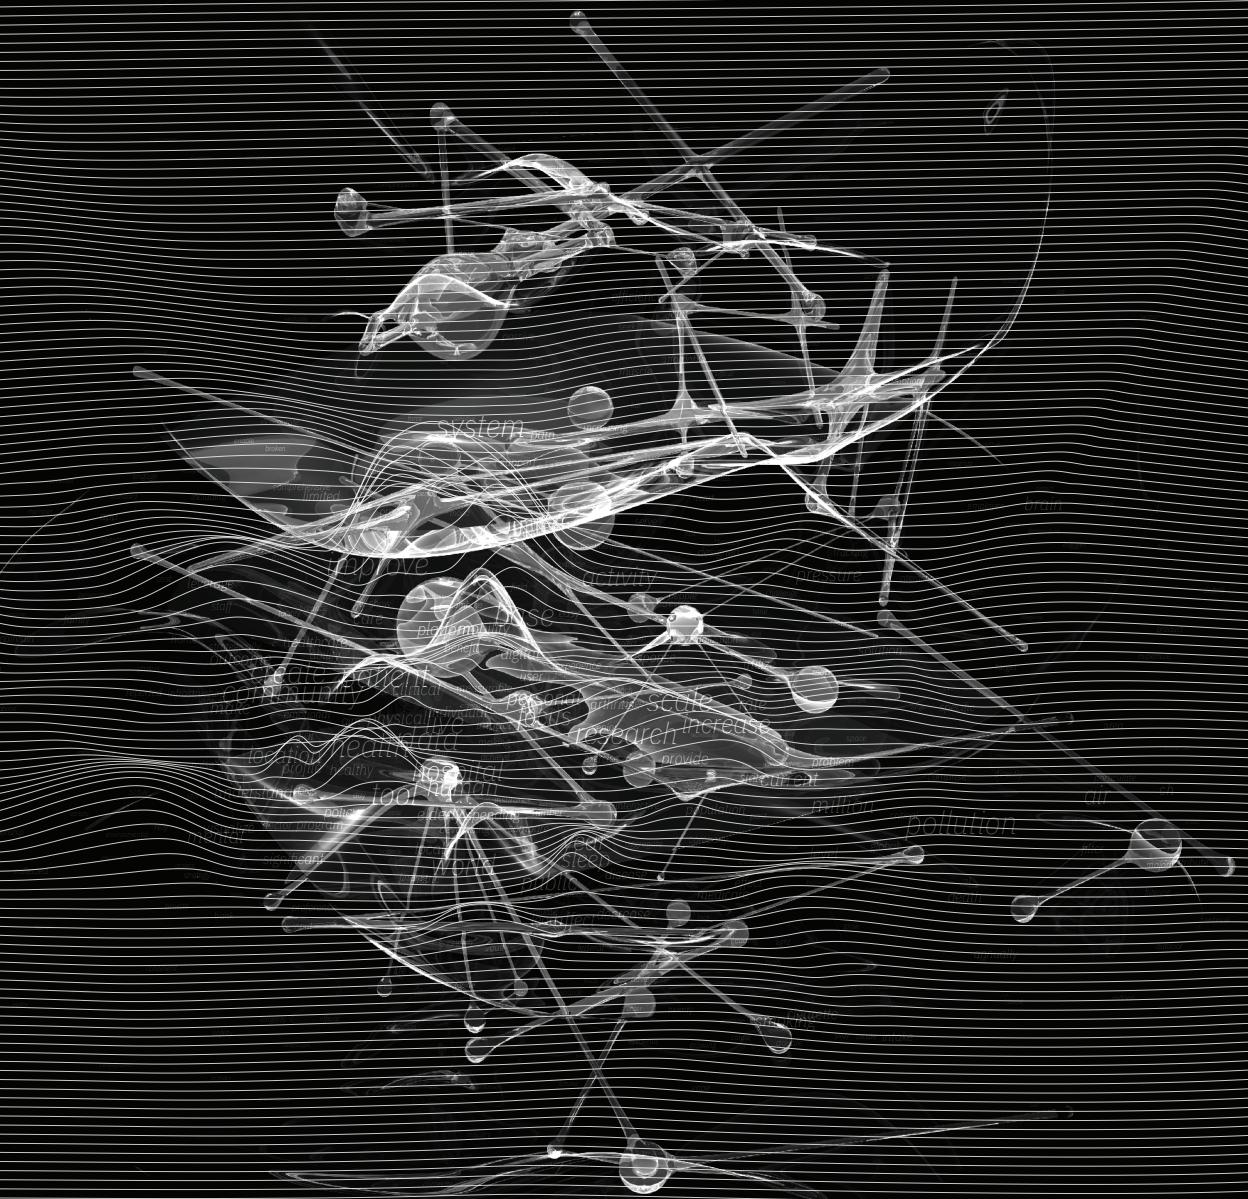

Master in Design Engineering at Harvard *Collaborative Studio* Volume 1 (2017-2018)

OPENING

| | |
|-----------------------------------|---|
| FROM THE EDITORS | 1 |
| In Celebration of Interstitiality | |
| ANDREW WITT | 3 |
| Designing Across Disciplines | |
| JOCK HERRON | 5 |
| The Topic of Health Systems | |
| FAWWAZ HABBAL | 7 |
| The Design Engineering Pedagogy | |


SELF 10

| | |
|--|----|
| NILE | 11 |
| Maintaining health and social connection in old age | |
| APEIROGON | 25 |
| Localized mental health spaces for the 21st century | |
| AMBLE | 31 |
| Nerve and muscle stimulation garment for chronic arthritis | |
| WITHIN SMOKE | 37 |
| Smoking's impact on private and public health | |

PATIENT 40

| | |
|--|----|
| AFIA | 41 |
| Affordable, fast, intuitive, accurate viral STI testing | |
| CODA | 55 |
| A therapeutic palliative care sanctuary for hospice patients | |
| OLIVE | 61 |
| Moisture-detecting smartbelt for ostomy care | |
| PAIR | 67 |
| The perfect pair of air shoes | |
| PHARMA 2100 | 73 |
| Global pharmaceutical funding | |

| | | | |
|---|------------|--|------------|
| <hr/> USER | 76 | <hr/> DIGITAL SELF | 142 |
| MALCOLM TEN | 77 | OMNI INDI | 143 |
| Enhanced data collection for pa- tient-reported outcomes | | Improving health outcomes with a multi-layered, data-driven digi- tal health service | |
| MOMENT | 91 | ATÉLIER | 157 |
| Focus training through a multi- sensory chair experience | | A creative agency, from your brain for your brain | |
| SYNCSENSE | 97 | REMESYS | 163 |
| Motion sickness mitigation system for air travel | | Reanimated emotional system | |
| MOBILIZE | 103 | INSOMNIGRAPH | 169 |
| A concealable exosuit for improv- ing walking efficiency | | A framework for visualizing and quantifying sleep patterns across time scales | |
| FLEXFIT | 109 | | |
| Socially connected physical ac- tivity for seniors | | | |
| ANOPHELINE VECTORS | 115 | | |
| Visualizing environmental change with longitudinal disease vectors | | | |
| <hr/> CITIZEN | 118 | <hr/> CLOSING | |
| NODE | 119 | FROM THE DIRECTORS | 171 |
| Reimagining emergency response for resilient cities | | | |
| CHÚ | 133 | STUDENT BIOS | 173 |
| Breathe fresh air everywhere | | | |
| HEALTHCARE | 139 | | |
| Spending vs. Outcomes | | | |

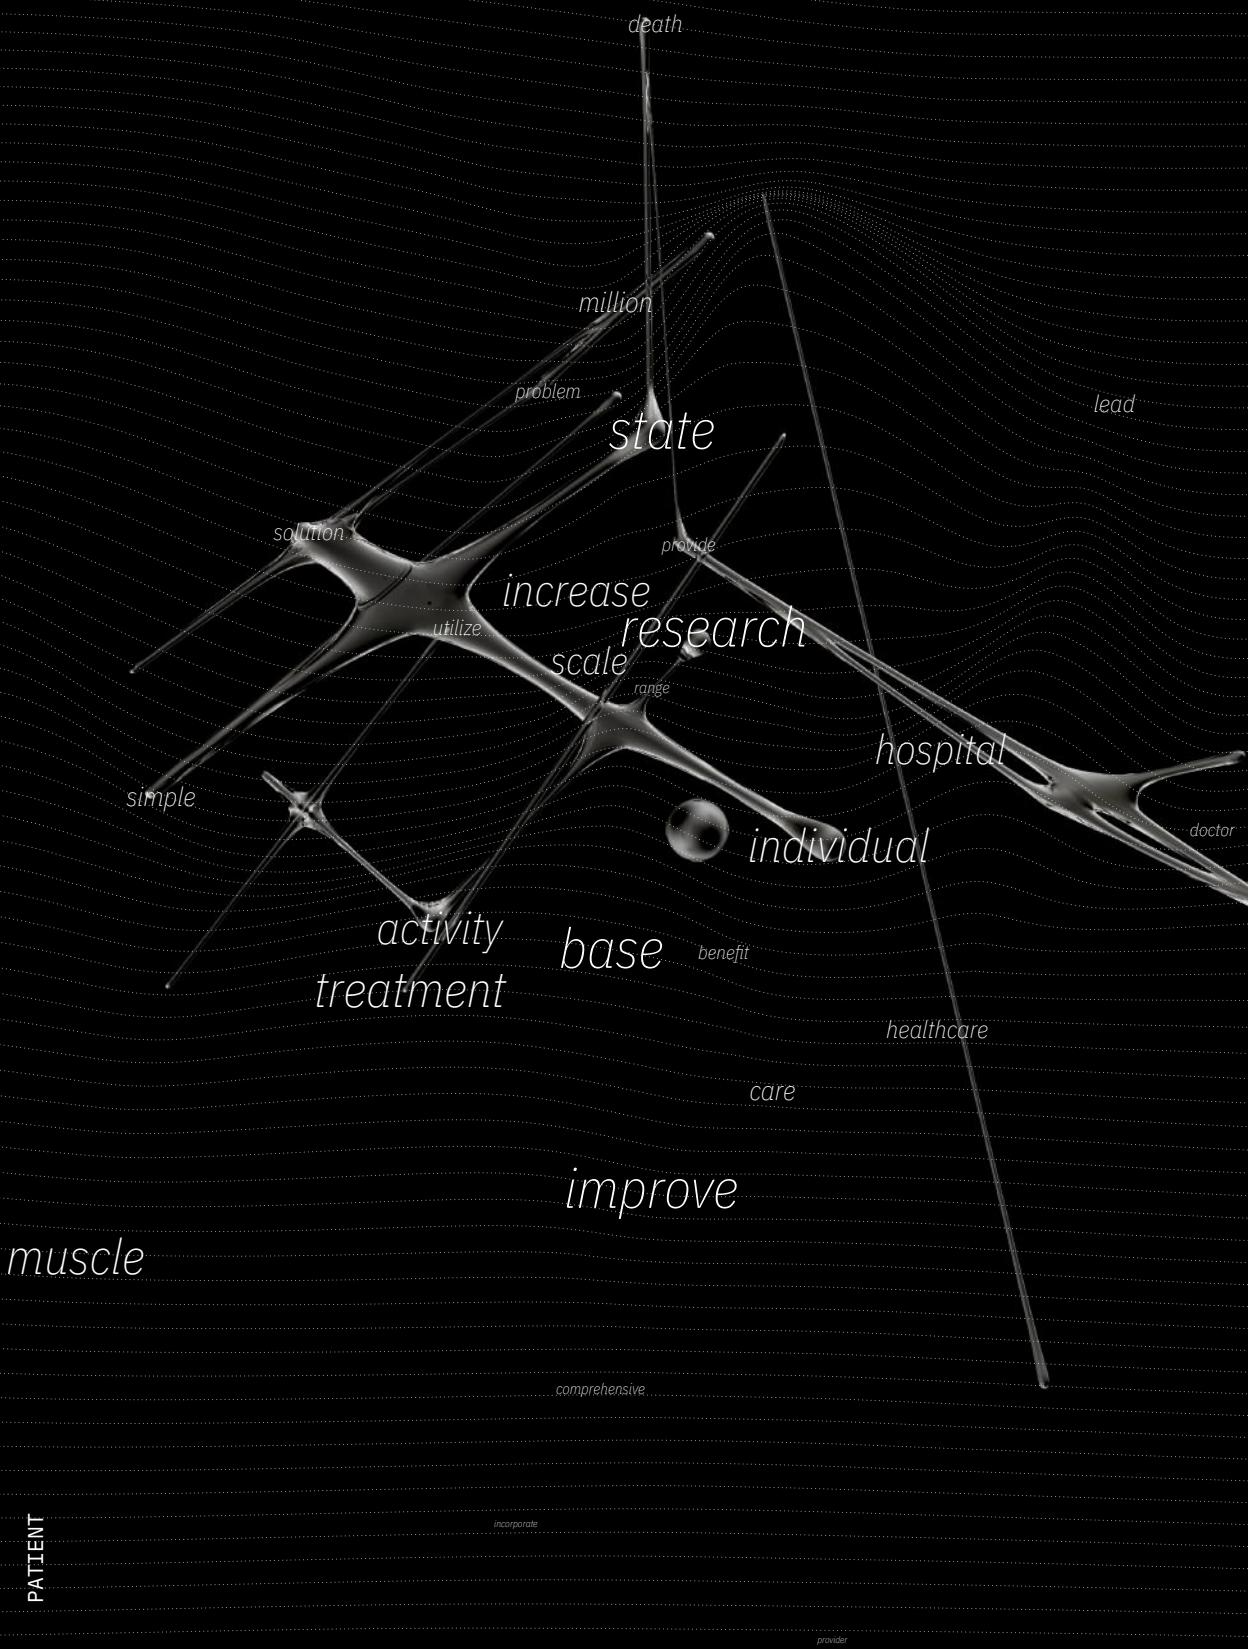

P

life

bank

connecting

PATIENT

How do I receive care? With the abundant data and resources available to inform decisions on our well-being, navigating the health system has become a burdensome task. These projects survey broad data and construct comprehensive pathways to better health outcomes to aid in answering the question: how and where should I, a patient, receive care?

P₁ AFIA

Affordable, fast, intuitive, accurate STI viral testing

P₂ CODA

Individualized therapy space designed to address mental health in the 21st century

P₃ OLIVE

A moisture detecting smart-belt for ostomy care

P₄ PAIR

The perfect pair of air shoes to correct gait and pressure for a better stride

P₅ PHARMA 2100

Mapping funding allocations of the global healthcare system to investigate the balance between preventative and chronic care

ABL
ACC
ACT
AIM
ALW
ART
BNF
BSE
CLN
CMM
CMP
CPH
CRE
CRR
CRT
CTC
CTY
CTY
DAT
DCN
DRC
DSN
DSS
DTH
DTL
DTR
DVC
EXP
EXR
FCS
FML
GEN
GTH
GVN
HLC
HLT
HMN
HPP
HSP
ICP
IMP
IMR
INC
IND
INF
LCT
LEV
LNG
LVE
LYR
MLL
OTC
PHY
PLL
PLT
PPL
PPU
PRC
PRJ
PRS
PRT
PRV
PSR
PTN
RSR
RTE
SCL
SLP
SMP
SNS
SPN
SPP
STT
SYS
TIME
TRK
TRM
TRT
UND
USR
UTL
VIS
VSN
WRL
YER

AFIA

*Affordable, fast, intuitive,
accurate viral STI testing*

37 million people in the world have HIV, and this number continues to grow. Diagnostic attrition is a major cause for concern in many parts of the world, a situation in which patients enter the diagnostic pipeline, but drop out of their testing schedule prior to receiving a final diagnosis. AFIA addresses this problem by reducing detection time for HIV infections via a field-deployable, low cost, standalone kit. Currently, patients who are interested in being formally tested and who are unaware of their condition do not take the steps necessary to get tested or treated (if necessary). Even though testing is not to blame for the epidemic, it does play a significant role in awareness, transmission, and patient agency. How can we increase patients' awareness of their condition and reduce attrition in a field of complex biological, medical, and regulatory constraints?

Julian Siegelmann, Kenneth So, Janet Sung, and Kiran Wattamwar



ABSTRACT

37 million people in the world have HIV, and number grows at the rate of millions per year. Attrition remains a problem where patients enter the diagnostic pipeline, only to drop out of their testing schedule before reaching a final diagnosis. The team aims to reduce attrition rates by reducing detection time for HIV infections. Due to a complex and strenuous diagnostic pipeline, many patients who are initially interested in a formal diagnosis lack timely feedback to inform steps toward treatment. Even though testing is not to blame for the epidemic, it does play a significant role in awareness, transmission, and agency. Current HIV testing may lack sensitivity to cost, is slow, and requires training, relegating it to expensive procedures often performed in labs. The need for sensitive testing is furthered by the "U=U" movement (undetectable = untransmittable), which was recently backed by the CDC. Given our market, regulatory challenges, and technical requirements, a good solution is (1) simple and intuitive, (2) fast, (3) deployable and easy to use in the field, and (4) affordable.

The team created a flow cytometry-based assay that implements microfluidic processes to safely, accurately, and quickly count viral load measurements in 1 mL of blood. The microfluidic device is implemented in concert with a companion app and phone accessory, which is designed to fit all standard phone types used in Africa and America. This allows both in-clinic and at-home usage. To circumvent the regulatory need for lab-based testing, the device is designed with simplicity and disposability in mind. The research and solution is presented here on four different scales: (1) the viral scale (technical interactions), (2) the device scale (components), (3) human scale (clinical and user experience), and (4) the systems scale (national rollout).

A PRIMER ON HIV

For HIV patients, there are multiple roadblocks to getting the care they need. Clinics in rural Africa are few and far between, leading to long travel times. Once at the clinic, congestion creates long wait times and patient anxiety, resulting in some parties leaving prior to receiving their test results. Currently, a patient who is interested in taking a test follows a rigid testing pipeline to confirm a positive diagnosis.

First, the patient must find a clinic. This alone can present a large barrier to those who live in rural regions or those who lack adequate access to healthcare funding to cover testing costs. Depending on available resources, clinics may lack the resources to service their patients. Additionally, the need for labs requires batch testing and formally trained clinical practitioners, leading to longer turnaround times.

Healthcare practitioners experience the same problems, but from a different perspective: centralized clinics may alienate patients farthest away from health centers, while also increasing patient load beyond capacity for a single point of access, leading to reduced patient/clinician time and elevated exposure to waiting room diseases. Additionally, costly lab equipment and batch processing mean tests cannot be carried into rural areas.

Furthermore, clinical testing is a densely regulated process that, under the regulatory framework of the Clinical Laboratory Improvement Amendments (CLIA) in the U.S., requires the clinics to hand over collected human biological samples to labs for sensitive medical testing. Clinics may not analyze samples themselves, and the submission of samples to labs introduces a significant amount of latency in communicating results back to patients.

These clinical barriers to HIV diagnostics have contributed to high rates of attrition in HIV screening. In order to speed up the diagnostic process, there needs to be a solution that can be safely performed at the point of care. To this end, an intervention that bypasses CLIA requirements is an essential design requirement.

Methodology


Background

The clinical screening process for HIV is staged and requires an array of sequential tests. Patients without known exposure to HIV will usually take the ELISA (enzyme-linked immunosorbent assay) rapid test first. The ELISA test checks to see if antibodies are present in samples collected from cheek swabs. The ELISA is cost-effective, non-invasive, and fast, but lacks enough sensitivity to determine a positive diagnosis. Patients with negative results drop out of the screening loop at this stage, and others continue with the more sensitive Western Blot test, followed by a Nucleic Acid Test (NAT). These tests are progressively more expensive and require incrementally more technical laboratory processes. NATs are the most precise test, with the authority to confirm a positive diagnosis, but they are also the most expensive in the screening process.

Advanced imaging tools and complicated lab procedures provide feasibility challenges that serve as bottlenecks in rural regions and under-supported clinics. Complicated devices with complex preparation processes, like NATs, which traditionally use gel electrophoresis, are difficult to deploy in remote clinics, where pocket-sized devices may be the most successful. Furthermore, devices must be resilient

↓ MICROFLUIDIC DEVICE

Below is an example of the AFIA microfluidic device, a new, proposed HIV test. Here, you can visibly see the effects of the mixer (the wavy portion of the design) that combines the chemicals from the wells, before forming small droplets. In reality, the diameter of these channels is 50 μ m, smaller than a human hair.

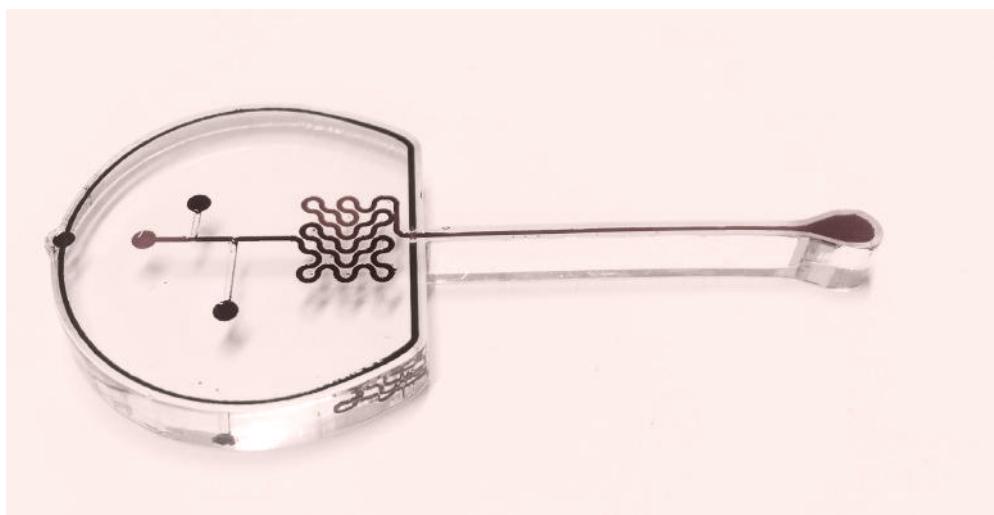

against dust and somewhat mobile to optimize for their usage in the field for clinics that travel (especially those that service rural regions).


These bottlenecks contribute to a grueling diagnostic process that requires patients endure the psychological burden of waiting, scheduling, and repeated planning. For clinics, regulations require the transfer of samples to labs for testing, creating a time crunch that compounds with a lack of adequate workers to address growing patient populations.

An optimal test given these challenges would be (1) affordable, (2) fast, (3) intuitive, and (4) accurate – AFIA. Affordable tests make individual testing rather than batch testing possible, which can incentivize point-of-care testing. Fast tests reduce the psychological burden on patients who must sit alone, anxiously waiting for results. Intuitive tests make on-site testing possible, instead of requiring labs to intervene. And finally, accurate tests can eliminate the battery of testing and offer a diagnosis from a single test.

In Arabic, “afia” means “good health.” This project, AFIA, embodies the above design principles as a framework for both evaluating the current HIV screening system and as a proposed clinical solution that could reduce attrition in patient diagnostics for HIV.

A New Testing Paradigm

While there are several intervention points in the system that could improve patient awareness of their HIV status, this project specifically focuses on HIV diagnostics. The diagnostics process itself is also broad, spanning improvements in patient experience to reductions in stigma, which can increase the volume of people who get tested. The team decided to address the shortfalls in the device utilized in testing for HIV. While improving the patient experience directly could ease the psychological burden of the process, we saw that addressing the problem at its root – a thorny series of tests – might offer a much larger scale solution for deployment in an array of clinics worldwide.

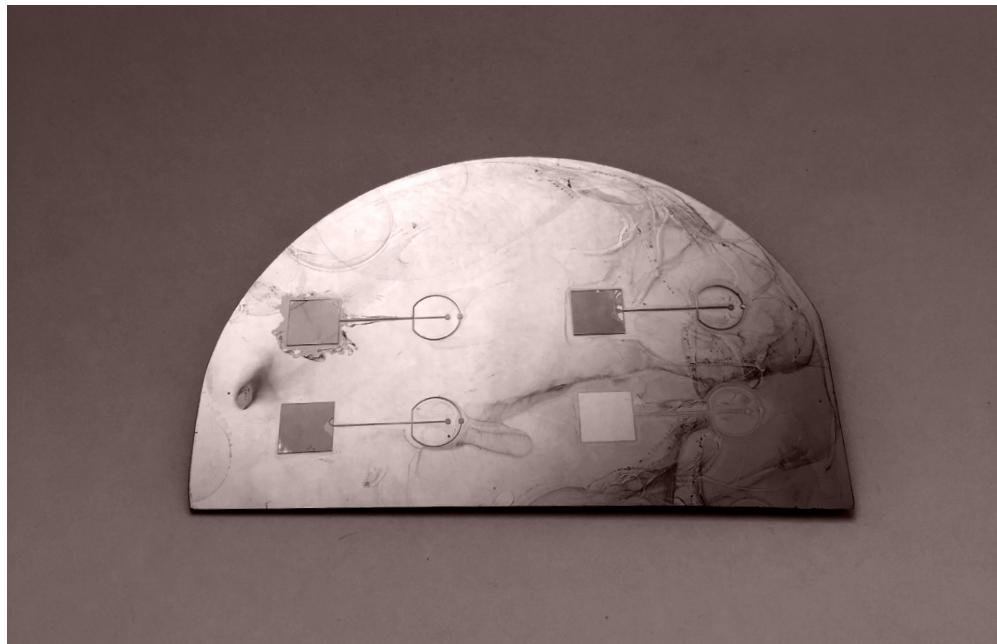


↑ AFIA, AT MICROSCALE

This plate serves as a template for testing the microfluidic design of AFIA's channels, bumpy mixers, and droplet former. The darker sections on the plate above have widths of 50um (smaller than a human hair). By pouring PDMS (a gel-like substance) above these raised sections, letting it set, and removing it, we form small channels and wells in the surface that are used as the base of our device. In that regard, this mask is a "negative" of the Afia device.

The team was also motivated by CDC's research with U=U (Undetectable = Untransmittable), demonstrating that HIV+ people with viral loads below 200 copies / mL cannot transmit HIV to someone else during exposure. While considering how to empower those managing HIV on a daily basis to understand their condition and transmissibility, the team also wanted to explore solutions that could measure viral load in the home. AFIA imagines a future where viral load testing can be performed the same way a diabetic might manage their sugar consumption by using a glucometer, which eliminated venous blood draws as a means of collecting blood samples.

Solution

Most existing HIV screening procedures do not meet the standards of affordable, fast, intuitive, and accurate. The team decided to take on the task of counting individual viruses, using a technique from droplet microfluidics. This technique can isolate single viruses and count them through fluorescent markers that attach onto the virus itself. The full solution is mapped in the schematic on the right, along with the corresponding components of the microfluidic device.

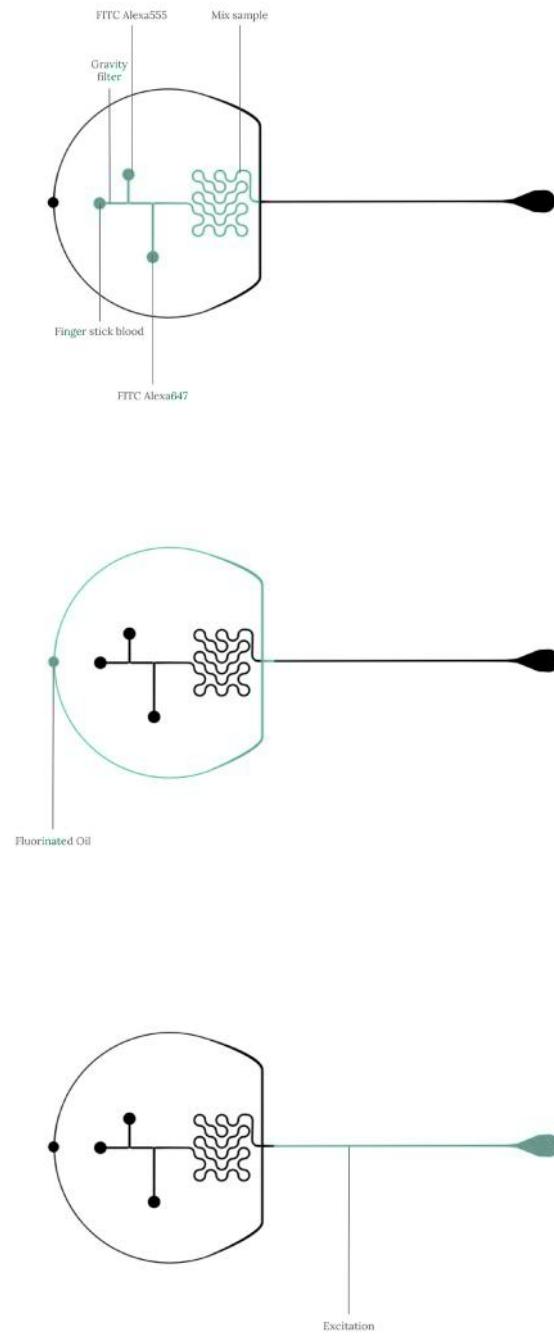

← STEP 1: COLLECT A SAMPLE

First, samples are collected using fingersticks, which plug into the microfluidic device. Plasma is extracted to reduce noise and prevent markers from binding to other parts of the blood sample. Along with this filtering, a pair of FRET markers that attach to HIV is introduced. FRET pairs fluoresce when they are close to each other. The team uses Alexa555 and Alexa647 antibody dyes conjugated to two nearby antibodies on HIV's surface to illuminate HIV (and only HIV).


The wavy pattern in the schematic is a mixer used to marry the chemicals in each well (circles) together.

← STEP 2: ISOLATE THE VIRUS

To count the virus' load, the viruses are separated into a single file line so that they can be imaged. This is done by flowing the mixture into a droplet generator geometry, a very small opening where a water-based and oil-based emulsion meet. By varying the flow rates of each, the team is able to generate bubbles of the water-based sample at a desired droplet size of 50um. The fluorinated oil functions as a spacer to keep the bubbles, or vesicles, separated. This droplet size is statistically likely to either have 0 or 1 copies of the HIV virus in it.

← STEP 3: DETECT + QUANTIFY

Using the excitation wavelengths and emission filters of the FRET pair, it is possible to excite each vesicle that passes a specially selected light. If the vesicle fluoresces, it contains a FRET pair and thus, contains a virus. The total count of fluorescent vesicles is a proxy for the viral load. To make this low cost and easy to deploy in the field, the design is an assembly that attaches to a cell phone, which then captures video of the droplets for processing.

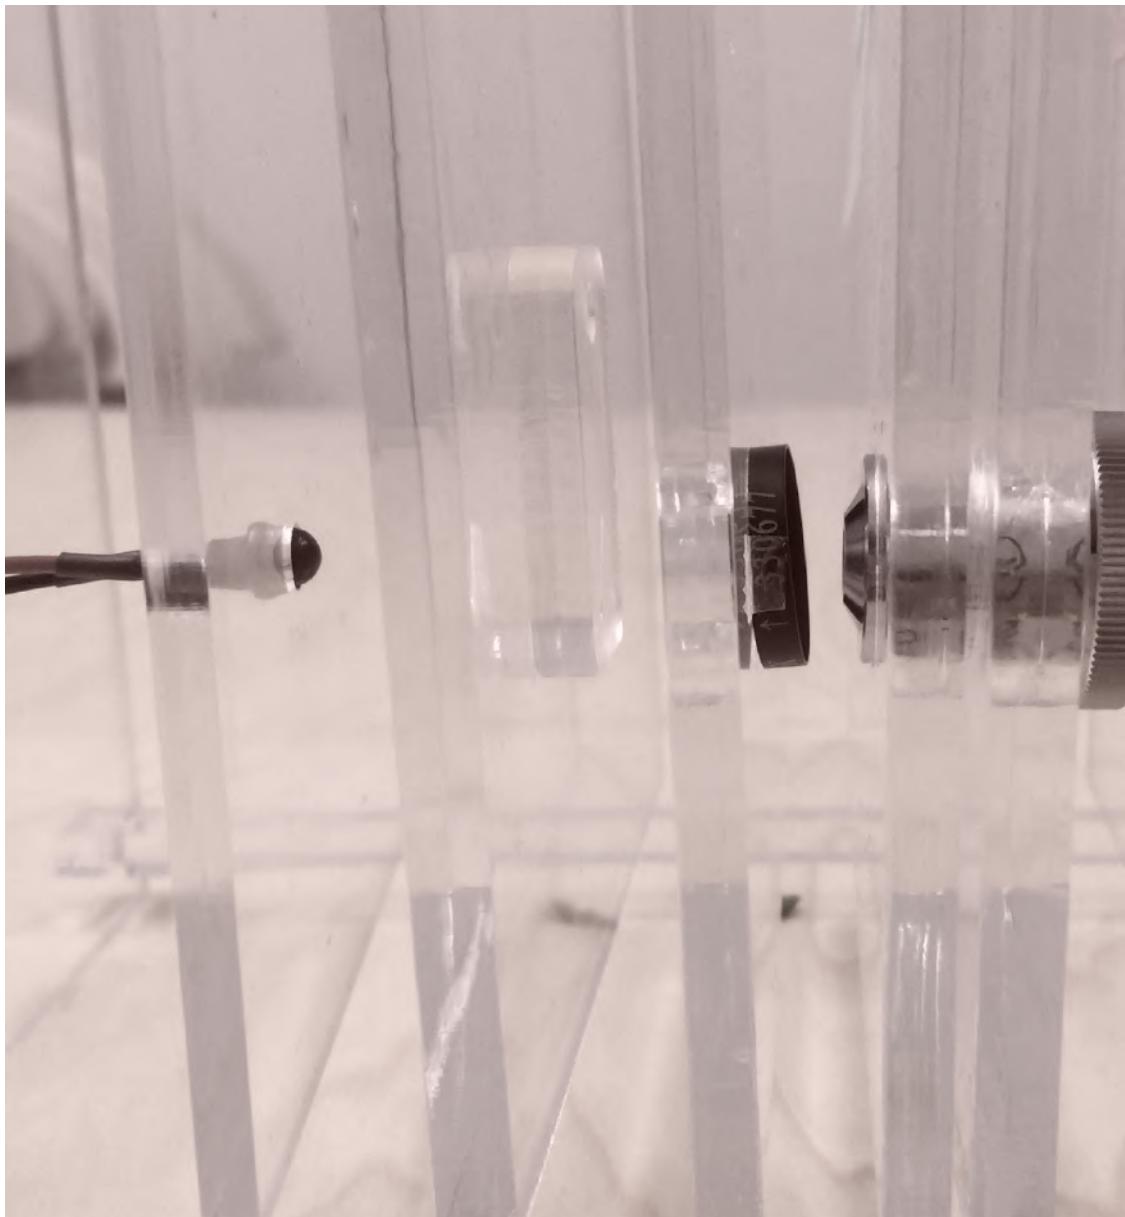

↑ LIGHTS, CAMERA, ACTION

This assembly represents the optical array. A light specifically makes FRET pairs visible, lenses focus on the viral scale, and filters specifically isolate fluorescent signals. The full assembly can allow a phone or microscope to see vesicles that contain viruses, and in turn, count the viral load of a sample.



Process

One of the biggest challenges in biology is the reproducibility of experiments. Given the variability in microfluidic implementations, the team thought through many of the nitty-gritty details to make the proposed solution both practical and feasible.

Using fluorescent markers, AFIA aims to capture fluorescence as a signal to mark that a virus is present. Organizing the signal emitted from markers is just as important as the ability to quantify it. An optical system with filter and lens is attached to the phone camera to remove environmental noise and amplify the correct fluorescent signal. By guaranteeing that vesicles have maximally one virus, an algorithm can count the binary signal and obtain the virus load of each sample.

Travelling clinics in the field require additional features: adequate lighting, protection from dust and theft, and portability. Because this work will likely not be done in a lab, the device must be easy to use, and adjusted to phones used in the regions in which AFIA is deployed.

The team explored several methods of prototyping and fabrication. Microfluidic devices are traditionally prepared by introducing engraved channels into some kind of base material. Many different ways to fabricate the device were considered, from laser cutting, to PDMS, to modular components that enable plug and play applications. Because the channels were around 50um, the team settled on PDMS.

Implementation

AFIA will be implemented in three stages: 1) in the clinical environment, to reduce the time needed to obtain results and reduce the number of uncollected results; 2) in the field, to allow mobile clinics and in-the-field healthcare workers to increase the number of HIV diagnoses; and 3) at home, to increase awareness regarding HIV viral load levels and empower patients to monitor their own health and transmission levels.


AFIA helps both patients and health practitioners by creating an affordable, fast, intuitive and accurate test that is portable and easily deployable in areas without clinical infrastructure. AFIA improves existing testing on two scales: 1), the physical scale, allowing the test to be deployable anywhere due to its lightweight and disposable nature; 2), in terms of interoperability, as this test can be used by anyone, eradicating the need for clinics and clinicians. This is extremely important, as increased access to HIV testing in rural areas decreases the amount of patients visiting centralized clinics for diagnostic and routine appointments, reduces the spread of diseases in waiting rooms, and reduces the number of patients leaving early due to uncomfortable and long waiting times. We can also roll this out to primary health entities in rural towns, providing accurate testing to even the most remote areas.

By making HIV tests more accessible and increasing the amount of patients that can be seen by doctors, we increase the number of HIV tests taken, reduce the number of uncollected results, and hope to create more transparency and understanding of viral load levels and treatment efficacy. This benefits both the clinic and the patient, both in Africa and the U.S..

We therefore aim to implement our solution within Africa and America first, creating a two-market strategy to monetize one market while subsidizing the other. In order to get our device onto the market, we have to (1) kick-off the medical certification process, (2) test implementation in rural markets, and (3) refine our market strategy to scale appropriately in both the U.S. and Africa.


↓ FULL DEVICE

AFIA is not only a microfluidic device, but also a full setup, that can be clipped onto a cell phone camera and covered to protect the imaging from dust when used on the field.

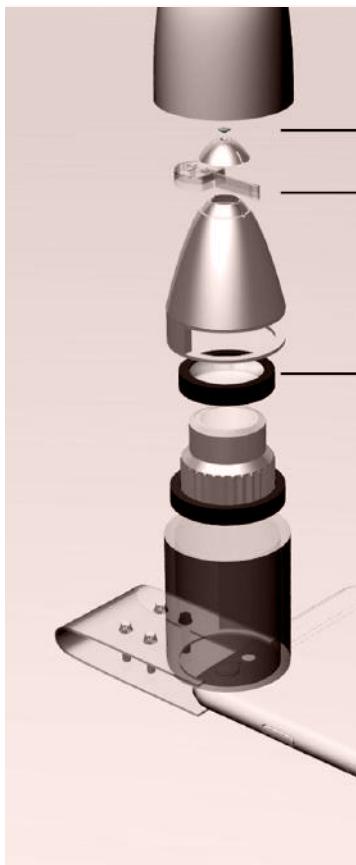

CONCLUSION

In implementing AFIA, we need to understand if we want to pursue public or private partnerships in the African market. Sadly, the NGO landscape can be dispersed and ineffective. A better option might be to work directly with governments. However, how can we ensure that our product does not get hampered by red tape and bureaucratic processes? Additionally, how can we incentivize health entities to implement AFIA? After speaking to experts, we understood that creating private sector profit established an appealing solution to implementation. Most importantly, how can we make testing a rewarding experience for the patient? HIV testing leaves both physical and psychological harm - pricking yourself isn't fun, and being reminded that you have HIV isn't either. There is still substantial work to be done to make HIV consumer testing a viable and desirable experience, but it is clear that advancing this technology development can advance the health and agency of a significant population in spades.

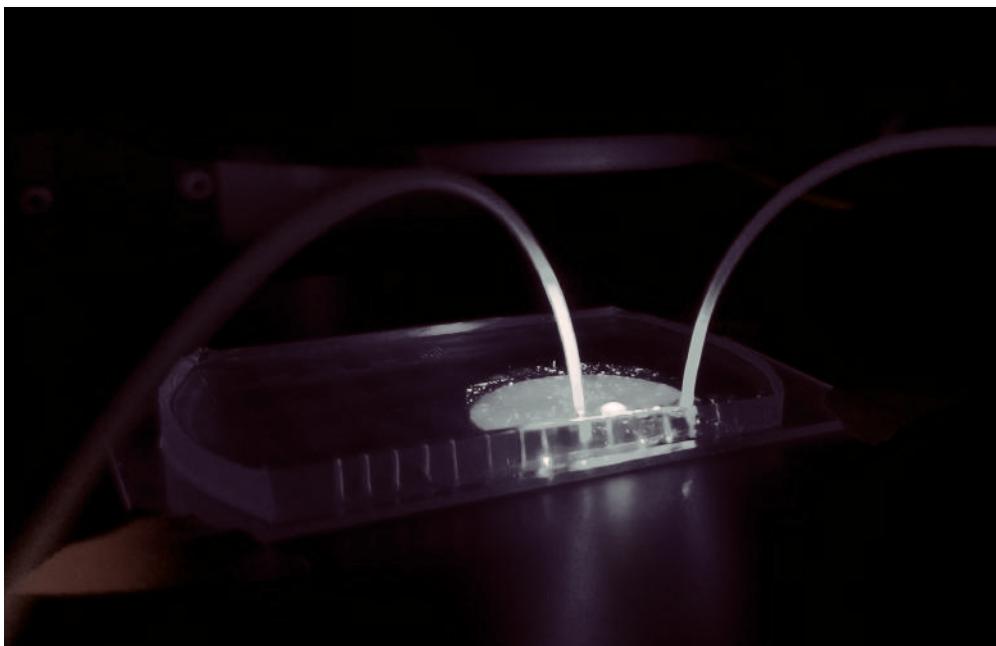

Interviews

Peter Stark, Harvard SEAS

Dr. Bruce Walker, Professor of Medicine at Harvard Medical School, Professor of Practice at MIT, and a Howard Hughes Medical Institute (HHMI) Investigator

Dr. David Knipe, Knipe Laboratory, Harvard Medical School

Dr. Hadi Shafiee, Principal Investigator, Assistant Professor in Medicine, Brigham and Women's Hospital, Harvard Medical School

Dr. Daniel Kuritzkes, Professor of Medicine at Harvard Medical School and Chief of the Division of Infectious Diseases at Brigham and Women's Hospital

Dr. Gio Traverso, MD, PhD. Instructor in Medicine, Division of Gastroenterology, Brigham and Women's Hospital, Harvard Medical School. Research Affiliate, Koch Institute & Dept. of Chemical Engineering, Massachusetts Institute of Technology

Galina Smith, Outreach Coordinator, The Boston Alliance for LGBT Youth (BAGLY)

Jordina Shanks, Chief Operating Officer, Planned Parenthood Massachusetts

Dr. David Weitz, Director of the Materials Research Science and Engineering Center

Melissa Hancock, Biological/Environmental Lab Engineer (INT), Harvard Medical School

Anas Chalah, Asst. Dean for Teaching and Learning, Director of SEAS's Teaching Labs

Christopher Hinojosa, Director of Discovery, Emulate, Inc.

Jason Robinson, IDEO

Dirk Ahlgren, IDEO

Christopher Wright, IDEO

Jeffrey Blander, CIO US Department of State

Darius Shahida, CFO, Butterfly Networks,

John Didier, Weitz Lab, Harvard University

Raoul Rosenthal, Lexiang Zhang, Postdoctoral Fellows

Walther Mothes, Professor of Microbial Pathogenesis, Yale School of Medicine

Alice Ly, Associate Director for Health and Sciences (H&S) at the Harvard Innovation Labs

Dr. Caleb Dresser, Clinical Fellow in Emergency Medicine, Beth Israel Deaconess Medical Center

References

- Promso S, Srichunrusami C, Utid K, Lulitanond V, Paijor W, Chanratita W. Quantitative detection of human immunodeficiency virus type 1 (HIV-1) viral load by real-time RT-PCR assay using self-quenched fluorogenic primers. *Southeast Asian J Trop Med Public Health*. 2006 May;37(3):477-87. <https://www.ncbi.nlm.nih.gov/pubmed/17120976>
- Cappy P, De Oliveira F, Gueudin M, Alessandri-Gradt E, Plantier J-C. 2016. A multiplex PCR approach for detecting dual infections and recombinants involving major HIV variants. *J Clin Microbiol* 54:1282–1288. doi:10.1128/JCM.03222-15.
- Janet M. Barletta, PhD, Daniel C. Edelman, MS, and Niel T. Constantine. Lowering the Detection Limits of HIV-1 Viral Load Using Real-Time Immuno-PCR for HIV-1 p24. *Antigenic American Society for Clinical Pathology. Microbiology and Infectious Disease / IMMUNO-PCR FOR HIV-1 P24 ANTIGEN 20 Am J Clin Pathol* 2004;122:20-27 20 DOI: 10.1309/529T2WDNEB6X8VUN
- Zeng et al., 2014 U. Zeng, X. Zhang, K. Nie, et al. Rapid quantitative detection of Human immunodeficiency virus type 1 by a reverse transcription-loop-mediated isothermal amplification assay *Gene*, 54 (12) (2014), pp. 123-128. <https://www.sciencedirect.com/science/article/pii/S0014480014000896#bbb0010>
- Barnor JS, Yamamoto N, Brandful JAM, Ampofo W, Bonney JHK, et al. (2014) Establishment of In-House Quantitative Real-Time RT-PCR Assay for HIV-1 Viral Load Measurement: Application to Evaluate Efficacy of ART in Ghanaian Patients in an Urban Setting. *J AIDS Clin Res* 5:305. doi:10.4172/2155-6113.1000305
- A. Orth, E. R. Wilson, J. G. Thompson & B. C. Gibson. A dual-mode mobile phone microscope using the onboard camera flash and ambient light. *Nature. Scientific Reports* volume 8, Article number: 3298(2018). 06 February 2018. <https://www.nature.com/articles/s41598-018-21543-2>
- Borghino, D. 3D-printed attachment turns smartphones into sub-wavelength microscopes, October 2013. <https://newatlas.com/3d-printed-smartphone-microscope/29340/>
- LaFratta CN, Huh SP, Mallillin AC, Rivello PJ, Walt DR. Visualizing Fluorescence: Using a Homemade Fluorescence "Microscope" to View Latent Fingerprints on Paper. *Journal of chemical education*. 2010;87(10):1105-1107. doi:10.1021/ed100290w.
- Tarver CL, Pusey M. A low-cost method for visible fluorescence imaging. *Acta Crystallographica Section F, Structural Biology Communications*. 2017;73(Pt 12):657-663. doi:10.1107/S2053230X17015941.
- Wei Q, Qi H, Luo W, et al. Fluorescent Imaging of Single Nanoparticles and Viruses on a Smart Phone. *ACS nano*. 2013;7(10):9147-9155. doi:10.1021/nn4037706. <https://www.ncbi.nlm.nih.gov/pmc/articles/PMC3951925/>
- Micahud, S. An Open Source Smartphone Microscope. *The Optical Society of America*. 06 December 2017. https://www.osa-opn.org/home/newsroom/2017/december/an_open-source_smartphone_microscope/
- Ngangue P, Bedard E, Zomahoun HTV, et al. Returning for HIV Test Results: A Systematic Review of Barriers and Facilitators. *International Scholarly Research Notices*. 2016;2016:6304820. doi:10.1155/2016/6304820.

Team Reflections


We were happy to dive deeply into a topic so technical and foreign to us. Our fresh eyes helped us approach and frame the problem with a unique perspective that doesn't often infiltrate this highly specialized space. We are so grateful to the incredible advisors who guided us through our process and the numerous clinicians, nurses, professors, researchers, and labs that offered us a glimpse into the many challenges and important lessons of HIV research.

Getting our hands dirty and really working on fabricating the device and learning additional lab techniques was immensely rewarding. The resources we were given and support to actually fabricate the microfluidic device made our project tangible and real. Early on, we chose to focus our efforts on tackling

the technical sides of our project, but realize that this came at the expense of the user experience journey. Nonetheless, we were able to use the insights gained from secondary sources to intuit pain points that our test could solve, and the next step would be to validate that with real users.

We deeply appreciated the opportunity to transcend barriers of academic disciplines and make full use of the resources given to us. By working very closely with studio professors and researchers who made the jump from academia to the private sector, we gained deep insight into how to transition from the lab to the real world. Every interview inspired clarity, learning, and technical expertise that we will carry forward with us as design engineers.



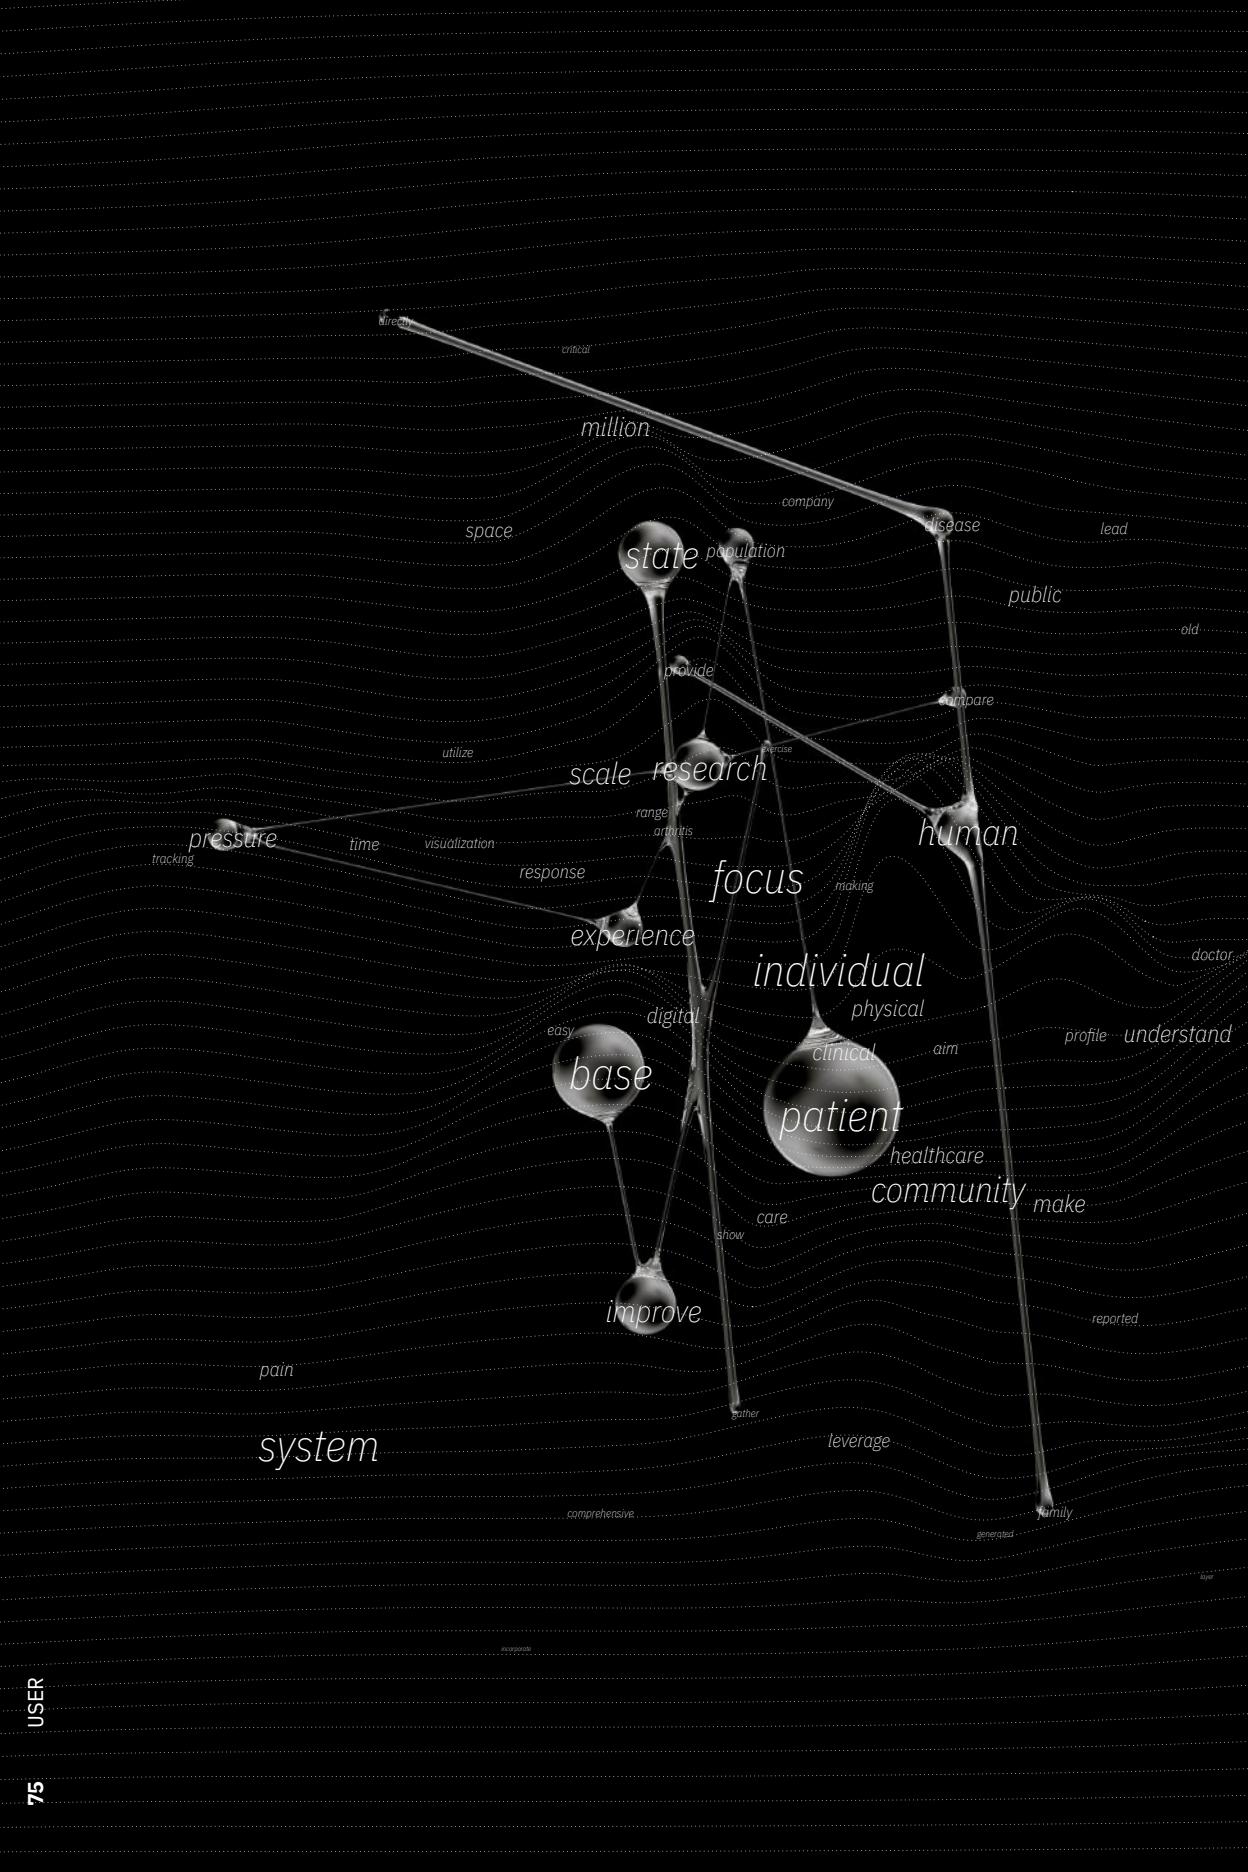

U

USER

How do I actively utilize resources?

At the center of products, platforms, and interfaces are users. As users, we are empowered to control the way we experience the world around us. With human centered design and studies on the impact of design decisions, these projects begin to understand the role of users in informing health outcomes along specific issues in healthcare.

continued:

U₁ MALCOLM TEN

An enhanced data collection platform for patient-reported outcomes

U₂ MOMENT

Focus training through a multi-sensory chair experience

U₃ SYNCSENSE

Motion-sickness mitigation for air travelers

U₄ MOBILIZE

A comfortable, concealable, affordable exosuit for assisting arthritic patients

U₅ FLEXFIT

A fitness ecosystem supporting seniors and their families with physical activities

U₆ ANOPHELINE VECTORS

Visualizing environmental change with longitudinal disease vectors

ABL
ACC
ACT
AIM
ALW
ART
BNF
BSE
CLN
CMM
CMP
CPH
CRE
CRR
CRT
CTC
CTY
CTY
DAT
DCN
DRC
DSN
DSS
DTH
DTL
DTR
DVC
EXP
EXR
FCS
FML
GEN
GTH
GVN
HLC
HLT
HMN
HPP
HSP
ICP
IMP
IMR
INC
IND
INF
LCT
LEV
LNG
LVE
LYR
MLL
OTC
PHY
PLL
PPL
PPU
PRC
PRJ
PRS
PRT
PRV
PSR
PTN
RSR
RTE
SCL
SLP
SMP
SNS
SPN
SPP
STT
SYS
TME
TRK
TRM
TRT
UND
USR
UTL
VIS
VSN
WRL
YER

MOMENT

*Focus training through
a multi-sensory chair
experience*

Moment is a multi-sensory chair aimed to help individuals with Attention-Deficit/Hyperactivity Disorder (ADHD) develop their ability to focus. Inspired by research showing that individuals with ADHD have a lower ratio of beta-to-theta brainwave activity when compared to the general population, the Moment chair targets this disparity and creates both a physical space and a digital interface to improve an individual's ability to focus. When a user engages with Moment, an array of sensory stimuli are activated, allowing for beta-to-theta brain activity to be affected. With meditative breath-rate visualization, scent, light, and sound, the Moment chair offers an oasis from distraction and a ritual to train your mind.



Nicki Adler, Saad Rajan, and Kiran Wattamwar

↓ AN OASIS FOR FOCUS

Moment is a multi-sensory chair designed for a holistic therapy experience for anyone along the attention spectrum. The system is thoughtfully designed to consider ergonomics, cognitive states, multiple sensory inputs, and lifestyles to create a ritual of focus.



MOMENT

Problem



Moment is a multi-sensory chair aimed at helping individuals improve focus, as based on neural activity models of populations with Attention-Deficit/Hyperactivity Disorder (ADHD). Research indicates that individuals with ADHD have a lower beta-to-theta brainwave activity ratio compared to the general population during periods of intense focus. Based on this cluster of studies, the Moment chair hypothesizes that inducing brain activity to match the general population's will improve an individual's ability to focus.

In a world of incessant notifications, infinite access to information, and addictive media baked into daily life, society's collective ability to concentrate is eroding. These phenomena, combined with pressure to boost cognitive performance, have led to record use of addictive stimulant drugs like Adderall and Ritalin. Moment counteracts the distraction and distress of modern times as a drug-free method of boosting performance and concentration. It ultimately seeks to help society control its reactions to ever-increasing stimuli. The design concept aims to help users focus on the moments, projects, and relationships that are most important.

Solution

Environmental factors measurably impact one's well-being. By reversing the paradigm and calibrating the environment, there are ways to reclaim control over one's well-being. Inspired by global meditation practices and mindfulness rituals, and informed by measured focus patterns in the brain, the Moment chair provides an oasis from a busy day.

It is also possible to modulate brain activity (specifically, the beta-to-theta ratio) by presenting sensory signals to the user at specific target frequencies. Combining these key insights, the Moment chair utilizes an array of sensory stimuli to induce brain activity and includes neural sensors to measure that activity. With a series of aurally prompted breathing exercises, alongside a meditative breath-rate visualization, scent, and light, the Moment chair is a rich sensory experience and a training ground for improving focus. By shaping the chair with smooth curves, minimally intrusive technology, and the feel of a protective shell, Moment is both a sanctuary and a productive environment to affect one's state of mind.

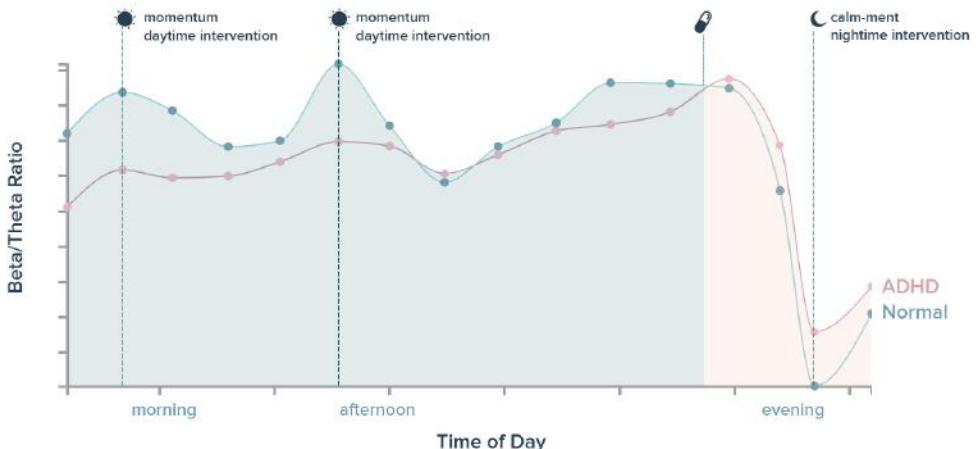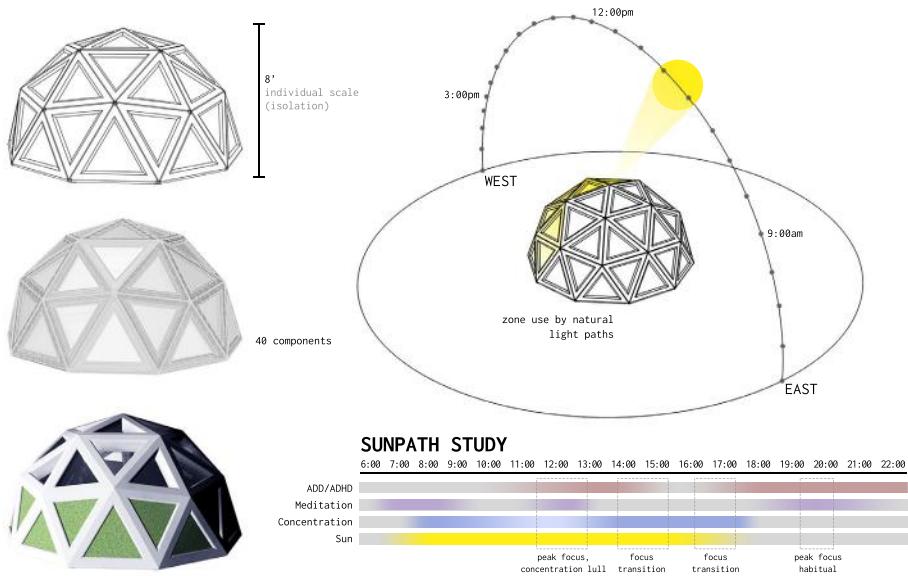

↑ SUNPATH STUDY (ABOVE)

As a device that can easily fit in one's office or home, the use of natural light can directly affect concentration or meditation levels. This study analyzes the impact of light throughout the day.



↑ SCHEDEULE (BELOW)

The beta and theta waves of people with ADHD vary throughout the day at a different rate than normal rates. Theta waves are associated with daydreaming, and beta waves are associated with focus. Moment facilitates intervention points to promote momentum and enervation in daytime focus activities, or "calm-ment" at night to help wind down the day.

↓ BIOMETRIC CALIBRATION

The user's breathing rate and brain activity together determine the breath-rate activity, where targets are adjusted and the visualization updates in real time. To accompany changing brain activity and breath-rate targets, sensory elements like sound, scents, and light are activated at certain frequencies. The technical diagram below shows the integrated feedback mechanism for biometric calibration.

Moment collects user data during the programmed exercises to measure how the programming is affecting brain activity in real time, and adjusts the activity (for example, target breath rate) accordingly. The feedback loop allows for each session to be individually tailored for each Moment experience. Despite its technical foundation, the Moment chair abstracts the technology, allowing for an organic user experience. From the anatomical curves to the raw wood, Moment is designed to immerse, relax, and captivate. The sensory elements of the chair (light, aromatherapy, sound, and visual cues) are informed by research on their impacts on state of mind, but also by time-tested cultural traditions. Most importantly, Moment is centered on a user's individuality, adjusting its programming for unique brain activity profiles, routines, and functions, all available as a daily ritual.

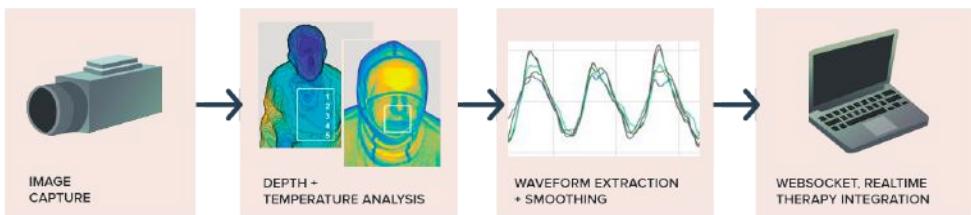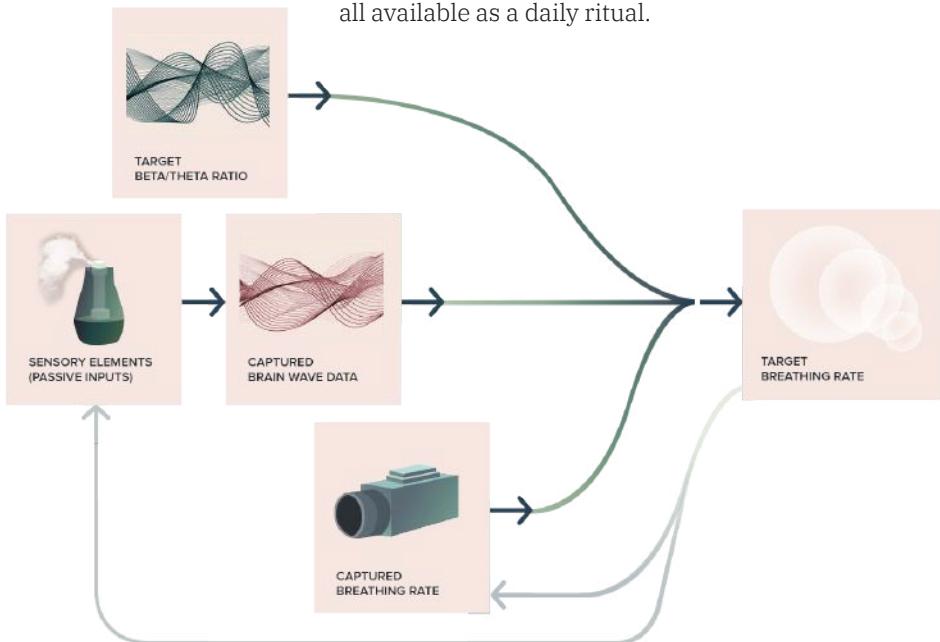



↑ CNC-MILLED CHAIR

The physical body of the Moment chair is the composite of several 2-dimensional cuts of wood made by a CNC mill. Assembled together, the Moment chair's contours represent a wave with smooth lines that mimic the sensory elements and breathing task integrated inside it. Aside from the physical body, the chair also features an embedded projector and a smooth surface covering the interior of the hood, which is where the breath-rate activity is projected within the chair. Inside the head cushion rests the body of a brain activity monitor, and additional components that users can attach to their temples to get a reading of their brain activity, while a detached FLIR camera captures their breath rate by monitoring temperature changes near the users' nose or mouth.

References

1. Journal of Attention Disorders, "A Decade of EEG Theta/Beta Ratio Research in ADHD"; American Psychiatric Association.
2. Children and Adults with Attention-Deficit/Hyperactivity Disorder (CHADD 2017)
3. Pereira, Carina Barbosa et al. "Remote monitoring of breathing dynamics using infrared thermography" Biomedical optics express vol. 6,11 4378-94. 16 Oct. 2015, doi:10.1364/BOE.6.004378
4. Procházka, Aleš et al. "Microsoft Kinect Visual and Depth Sensors for Breathing and Heart Rate Analysis" Sensors (Basel, Switzerland) vol. 16,7 996. 28 Jun. 2016, doi:10.3390/s16070996
5. Mott, M. S., Robinson, et al. (2012). Illuminating the Effects of Dynamic Lighting on Student Learning.
6. Nature, Dellacherie, D., et al. (2017). "Children and adults with Attention-Deficit/ Hyperactivity Disorder cannot move to the beat."
7. Sowndhararajan, K., et al. (2016). "Influence of Fragrances on Human Psychophysiological Activity: With Special Reference to Human Electroencephalographic Response." Scientia Pharmaceutica
8. NCBI, Moore, A., Gruber, et al. (2012). "Regular, brief mindfulness meditation practice improves electrophysiological markers of attentional control";
9. Desai, R., et al. (2015). "Effects of yoga on brain waves and structural activation: A review. Complementary Therapies in Clinical Practice"
10. Australian Journal of Educational & Developmental Psychology "Biofeedback and Children with ADHD";
11. New York Academy of Science, "Alternative treatments for adults with attention-deficit hyperactivity disorder"

MOBILIZE


A concealable exosuit for improving walking efficiency

Mobilize is a comfortable, concealable, and affordable exosuit for increasing muscle efficiency and decreasing joint pain while walking. While walking is already an extremely efficient process handled by the human body, muscle movements can still be used to activate external systems like passive exoskeletons to make walking even more efficient.

Using auxetic springs that work to complement muscle movement, the Mobilize exosuit uses a tensile structure to support walking. In parallel, the suit uses rigid structural elements to support joints, providing structure and compression. Together, these elements assist with muscle movement and joint pain, two major pain points for arthritis patients. An affordable, discrete, wearable device can improve mobility for a wide range of people who do not want their mobility constraints to be visible to others through the use of canes or walkers. Mobilize lets users take dignity and strength in their strides.



Jeronimo Beccar, Arjun Menon, and Kiran Wattamwar


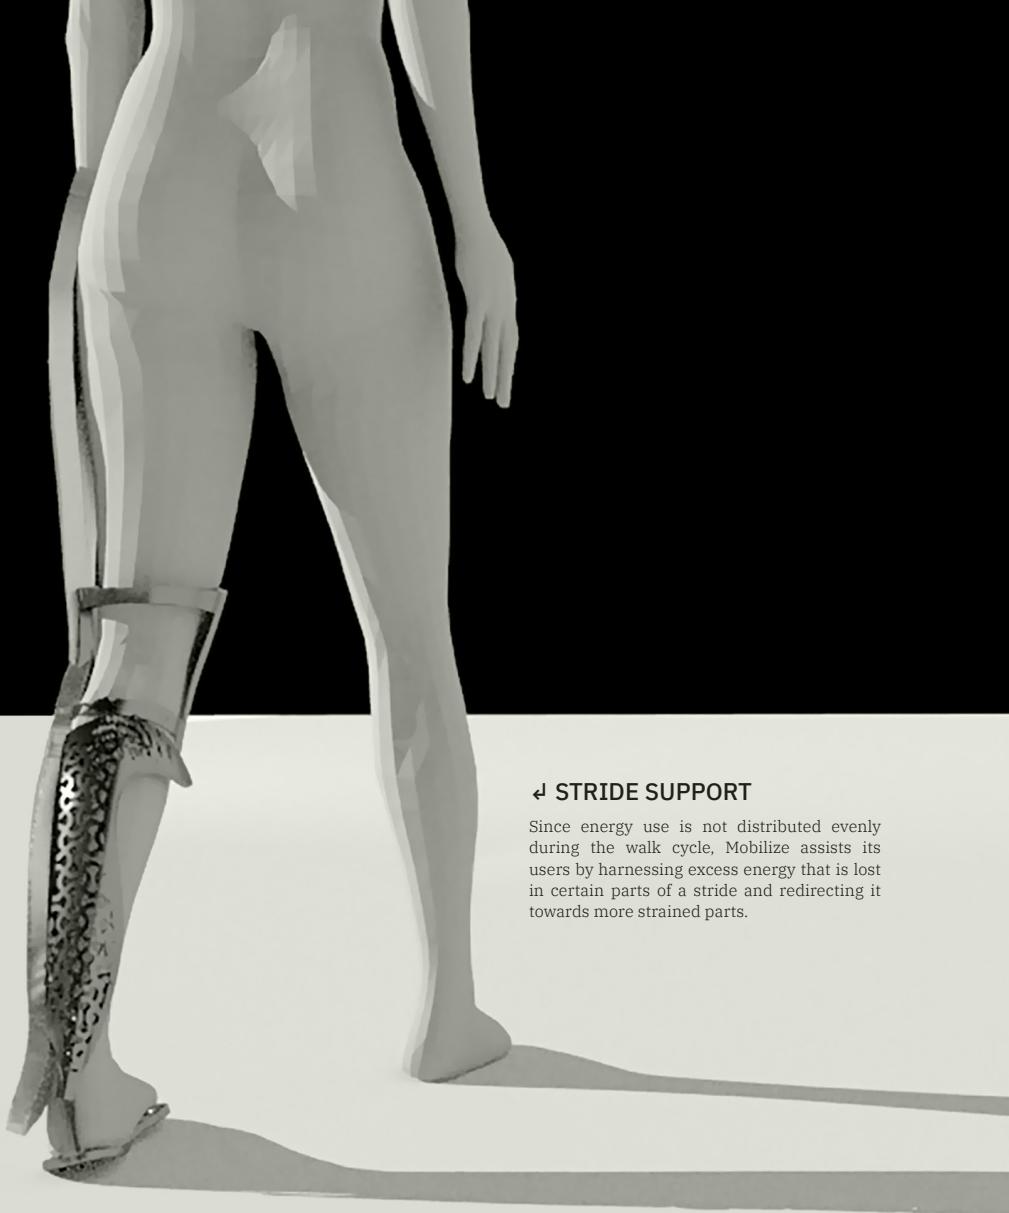


↳ STRIDE SUPPORT

Since energy use is not distributed evenly during the walk cycle, Mobilize assists its users by harnessing excess energy that is lost in certain parts of a stride and redirecting it towards more strained parts.



Mobilize

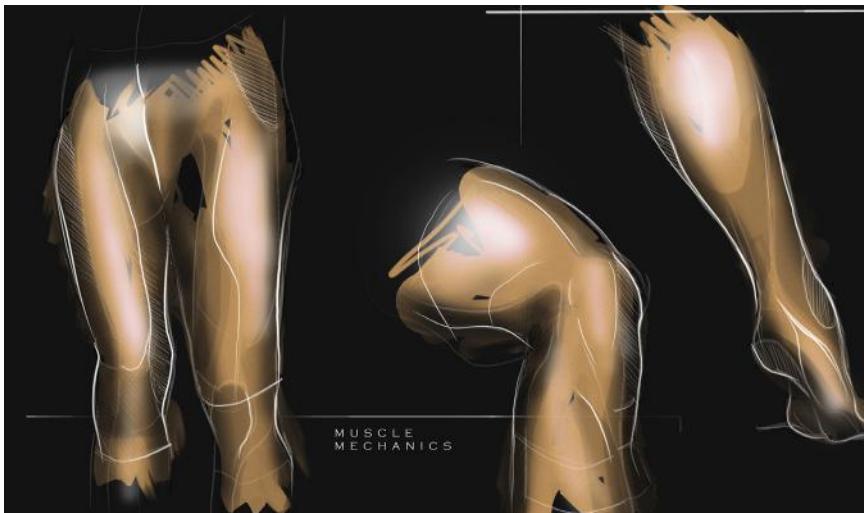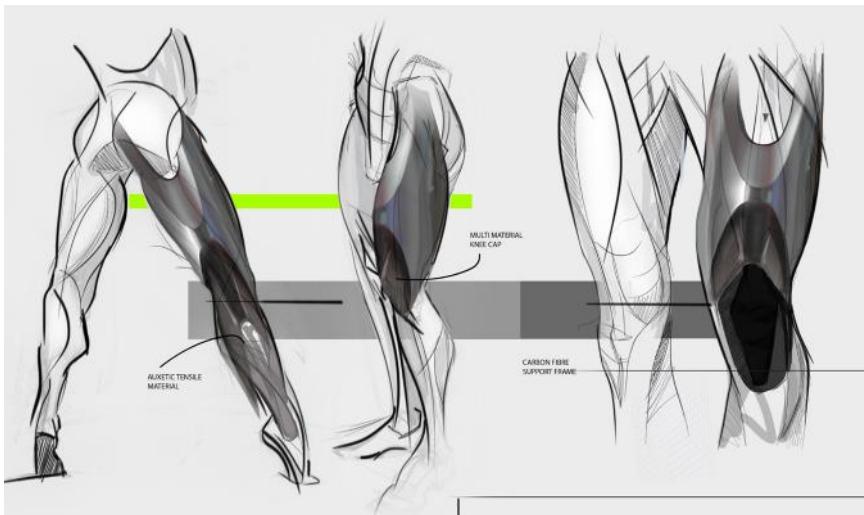

Problem

More than 50 million adults have already been diagnosed with some form of arthritis within the U.S. (Arthritis Foundation). Walking is an essential part of mobility for members of aging America, but even the simplest of actions become painful and difficult for those with arthritis.

Many exosuits designed to reduce the load (and therefore strain) on a wearer have been in development, but they are made with rigid materials that are meant to be worn on the exterior of a person's clothes. These are not easy to integrate into daily lifestyles with dignity, and are not seamless.

Exosuits currently on the market are primarily targeted towards defense and factory applications, with little focus on most of the population battling the consequences of arthritis. Other products currently address the needs of arthritis patients separately, without integrating them into a single system. Partial solutions like compression garments (usually designed for athletes), spring shoes, canes, pain medicines, and therapies for muscle development are difficult to weave into a single consumer product that performs well.

Usually, these needs are not combined into all-purpose systems that are truly integrated and effective in increasing muscle efficiency. Without a viable market solution to appeal to the mass market, sufferers of arthritis look to temporary relief solutions or drastic changes like surgeries and medication rather than seeking external aids that can continue to keep people mobile and active.

↳ EXPLORATION PROCESS

The core of this project rests on its materiality – from comfort to effectiveness, the success of a wearable exosuit meant for the masses depends entirely on its attention to detail in choosing the right materials.

Relying on materials like tensile polymers, the team designed its own auxetic stretchy materials, shaped by the contours of the human leg and calf muscles, to function as a spring in the tensile mechanism. This was cast in silicon with a custom mold, as a first pass.

Because this section of the garment was meant to support and mimic human musculature and increase muscle efficiency, this auxetic spring was tested for tensile properties like shore hardness, and compared to what was recorded by other academic research focused on muscle efficiency with passive systems.

↳ MATERIAL CONSIDERATIONS

The team investigated a collection of other materials, like stretchy fabrics, that could feasibly provide compression and comfort while withstanding daily wear, to construct the actual body of the suit.

Ultimately, Spandex was the best and most familiar option to users, which could make the garment integrate better into a daily wear cycle. Stiffer and supportive foams like Dela Foam and polyurethane foams were sewn into supports for a connected knee-brace, ankle brace, and shoe sole, to offer more compression and structural support in these areas where joint pain is the most prominent.



↑ FUTURE ITERATIONS

After performing a topology optimization on where the rigid supports would best be placed, the team considered the construction of rigid structural elements made of carbon fiber, which would offer a lightweight and thin shell to the areas of the exosuit that need a fixed structure. Other methods, like printing tensile materials directly onto fabrics to incorporate gradients of rigidity in a more streamlined way, might offer this exosuit more fertile ground in consumer applications in the future. Though the final suit was not realized in its intended form, the blueprints of the suit and its individual components offer promise that a wearable exosuit for arthritis patients is on the horizon.





Solution

The combination of a rigid support system and a tensile passive system can increase muscle efficiency, reduce joint pain, and promote better gait for patients with developing arthritis and decreased mobility. Mobilize aims to synthesize the benefits of orthotics, passive exosuits, and compression by focusing on soft, wearable materials. By using such materials, the Mobilize exosuit addresses its core design competency: the opportunity for concealment and daily use. Based on surveys with people with arthritis, it was evident that many people who could benefit from exo-suits do not consider them as options when choosing solutions to mitigate the effects of arthritis.

Canes and walkers fall within the same category, because they are not concealed and reduce the user's dignity. With a strong focus on material, the Mobilize exosuit is stretchy in areas of expansion and rigid where the body does not compress or expand. This combination accommodates movement but provides compression along joints to reduce pain. Guided by research in academia, the tensile structure and clutch redistribute energy along the walk cycle to increase muscle efficiency. Finally, the Mobilize exosuit incorporates a multi-material injection molding of stiff and flexible polymers that is applied directly onto the garment's base layer to increase comfort for users.



References

1. US Figure for 2017, by the Arthritis Foundation, 2017 Annual Report <https://www.arthritis.org/Documents/Sections/About-Arthritis/arthritis-facts-stats-figures.pdf>
2. Kuder, Izabela & Arrieta, Andres & Raither, Wolfram & Ermanni, Paolo. (2013). Variable stiffness material and structural concepts for morphing applications. *Progress in Aerospace Sciences*. 63. 33–55. 10.1016/j.paerosci.2013.07.001.
3. <https://doi.org/10.1016/j.paerosci.2013.07.001>
4. Smardzewski, Jerzy & Kłos, Robert & Fabisiak, Beata. (2013). Design of small auxetic springs for furniture. *Materials and Design*. 51. 723–728. 10.1016/j.matdes.2013.04.075.