


York - Chemistry - Mass Spectrometry Service Report

kat 1.19

Analysis Information

Acquisition Date 03/02/2017 16:06:41

Analysis Filename dks62964kt_P1-E-5_01_2613.d
 Method 600p_lcms_2c1s.m
 Submission Name dks62964kt
 Instrument micrOTOF
 ESI Positive

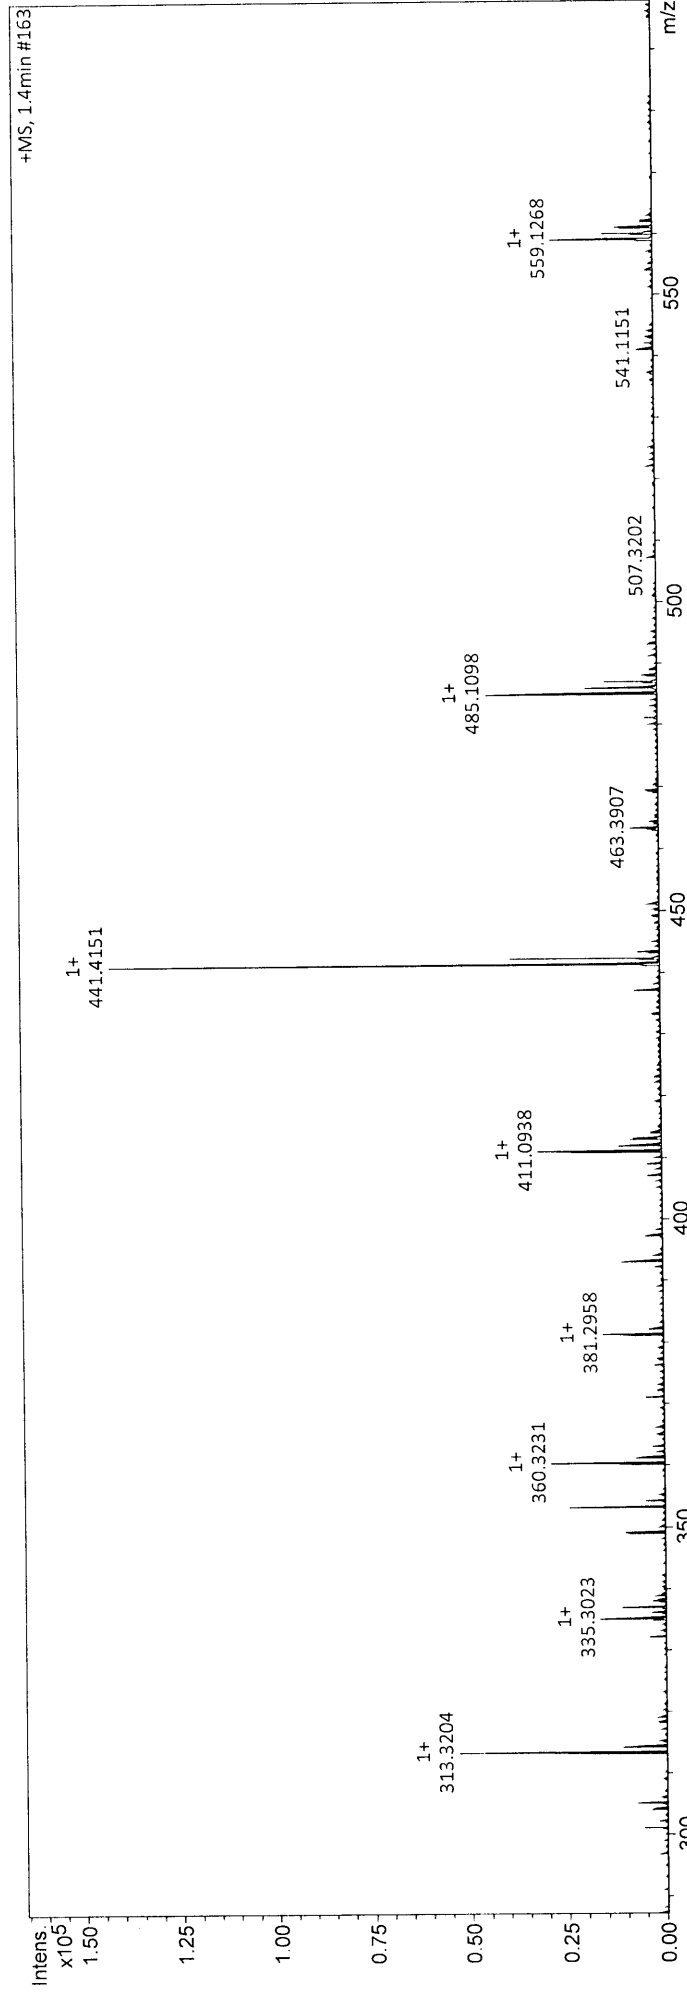

Meas. m/z	#	Ion Formula	m/z	err [ppm]	err [mDa]	mSigma	Mean err [ppm]
441.415131	1	C ₂₅ H ₅₃ N ₄ O ₂	441.416303	-2.7	-1.2	11.4	3.2