

York - Chemistry - Mass Spectrometry Service Report


KATI 1 L-Iys(Boc)2

Analysis Information

Acquisition Date

19/01/2017 12:46:52

Analysis Filename dks62691kt_P1-C-7_01_2233.d
Method 400p_lcms_2c1s.m
Submission Name dks62691kt
Instrument micrOTOF
ESI Positive

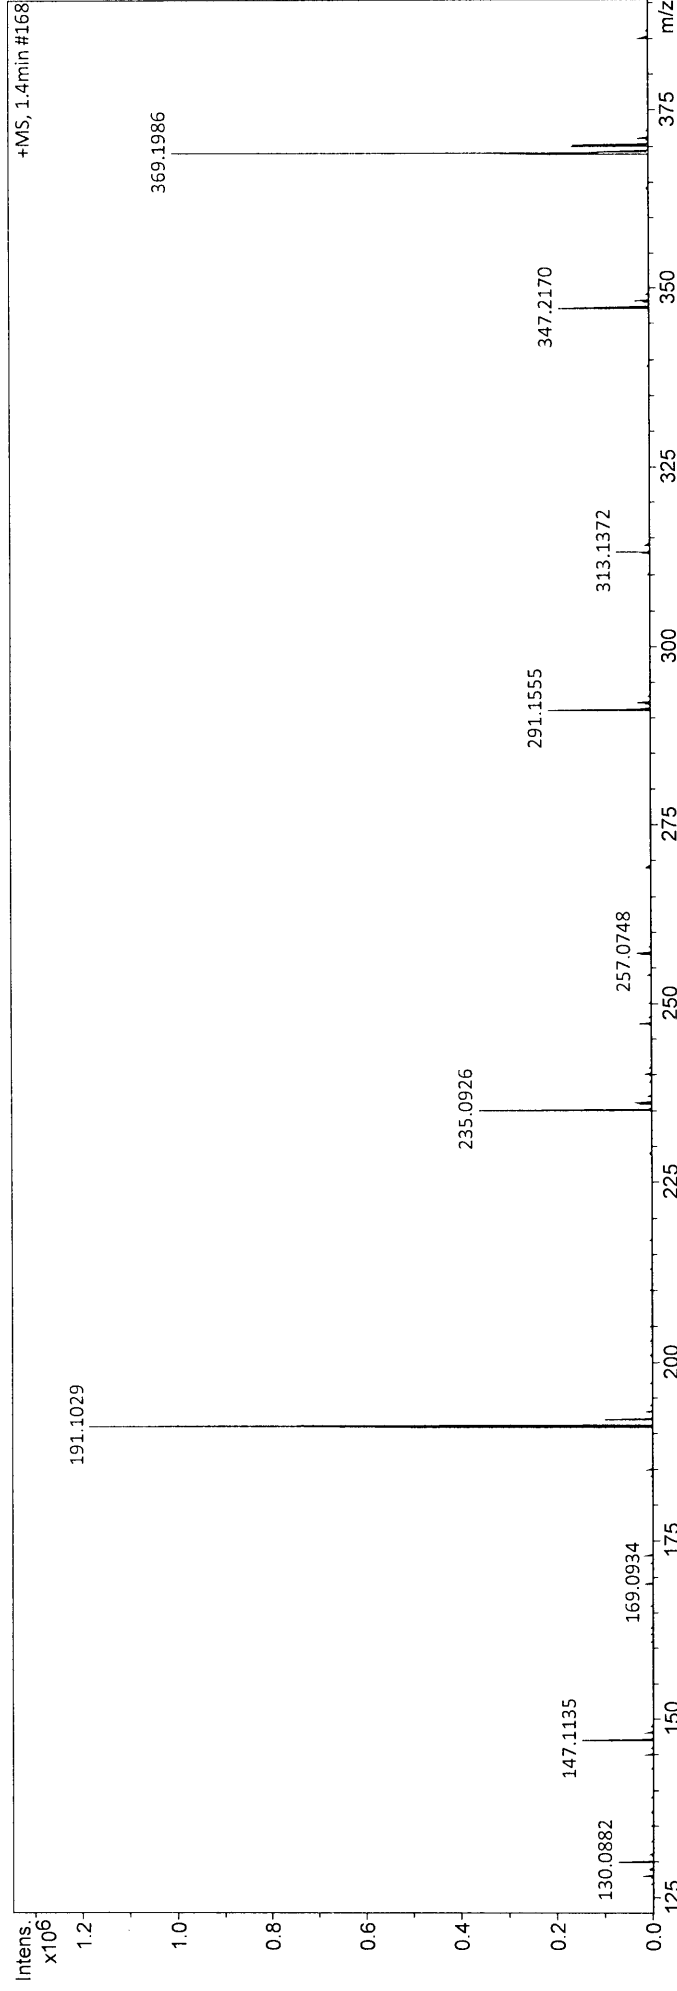

Meas. m/z	#	Ion Formula	m/z	err [ppm]	err [mDa]	mSigma	Mean err [ppm]
347.2170	1	C ₁₆ H ₃₁ N ₂ O ₆	347.2177	1.8	0.6	18.4	1.8
369.1986	1	C ₁₆ H ₃₀ N ₂ NaO ₆	369.1996	-2.8	-1.0	16.5	3.4