

Certificate of Analysis

Lab ID: **SS-083**

REPORTED September 21, 2026

CLIENT

VERIFY peptidetestcanada.ca/verify

EMAIL info@peptidetestcanada.ca

SCAN TO VERIFY



PTC-JDE9P73E

END CUSTOMER


NAME Matija-Skool.com/peptides

§ 01 Sample Information

FOR RESEARCH PURPOSES ONLY

Sample ID: **SS-083** Received: **09/11/2026**
Compound: **SS-31** Analyzed: **09/21/2026**
Report No.: **COA-2026-SC-01658** CAS: **736992-21-5**
Lot Number: **SS50-097** Formula: **C₃₂H₄₉N₉O₅**
Total Mass: **213.7 mg** Mol Weight: **639.4 g/mol**
Appearance: **Lyophilized powder**

SAMPLE PHOTOGRAPH

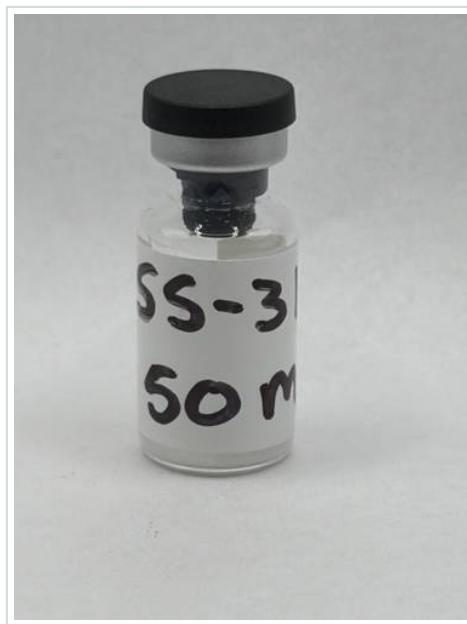

§ 02 Analytical Results

Qualitative and Quantitative chemical analysis by Liquid Chromatography Tandem Mass Spectrometry (HPLC-MS/MS)

	SPECIFICATION	RESULT	STATUS
Compound Test:	SS-31	SS-31	
Net Peptide Content:	50.00 mg	28.18 mg	
Peptide Fill Accuracy:	≥ 90 %	56.4 %	PASS
Chromatographic Purity:	≥ 98 %	99.7 %	

Peptide fill accuracy is the measured net peptide content expressed as a percentage of the declared label claim (measured ÷ label claim × 100).

Chromatographic purity is the target peptide's concentration as a percentage of the total peptide concentration measured — the target peptide against the other trace peptides detected in the same sample. It reflects peptide-related impurities only; it does not measure salts, excipients, or water, and is separate from net peptide content (the actual mg of peptide). — means not determined.

§ 03 HPLC-MS/MS Detail


METHOD A · AGILENT 1290 INFINITY II + 6495 QQQ · ESI+

PRECURSOR [M+2H]²⁺

320.70 Da

Quantifier transition ● MRM

320.70 > 120.10 CE 25 V

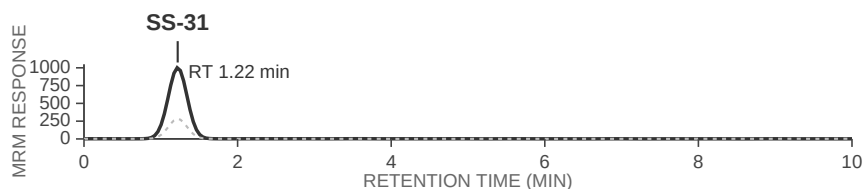

ROLE	TRANSITION	CE
● Quantifier	320.7 > 120.1	25 V

Agilent Poroshell 120 EC-C18 · 2.1×100 mm · 2.7 μm · Solvent A: 0.1 % formic acid in H₂O · Solvent B: 0.1 % formic acid in Acetonitrile

DISCLAIMER · RESEARCH USE ONLY

Results relate **only to the sample as received** by Side-Chain Analytics Inc. and the tests performed, as and when received — not to any other unit, vial, lot, or batch, and not to any other product bearing the same name, label, or description. This report is not a verification of any lot or batch. **For research use only:** this report is not a certificate of quality, safety, efficacy, or regulatory compliance; the material tested is not authorized by Health Canada for human or veterinary use; and this report is not for human or veterinary administration, clinical or diagnostic use, or label claims. Side-Chain Analytics Inc. does not manufacture, source, or sell the material tested and makes **no warranty, express or implied**; its liability shall not exceed the testing fee. This report may not be reproduced except in full, and may not be reproduced, displayed, quoted, or referenced — in whole or in part, including by any badge, seal, or link — in connection with the advertising, offer for sale, sale, or distribution of any product. This certificate is valid only as currently shown at sidechainanalytics.com/verify and may be withdrawn.



Certificate of Analysis

Lab ID: **ENDO-SS-035**

REPORTED September 10, 2026

CLIENT

VERIFY peptidetestcanada.ca/verify

EMAIL info@peptidetestcanada.ca

ORDER # PTC-32800

SCAN TO VERIFY



PTC-ZW8TM8D8

END CUSTOMER


NAME Matija-skool.com/peptides
PPHK

§ 01 Sample Information

FOR RESEARCH PURPOSES ONLY

Sample ID:	ENDO-SS-035	Received:	08/12/2026
Compound:	SS-31	Analyzed:	09/10/2026
Report No.:	COA-2026-SC-01318-EN	CAS:	736992-21-5
		Formula:	$C_{32}H_{49}N_9O_5$
		Mol Weight:	639.4 g/mol
Total Mass:	64.6 mg		
Aliquot mass:	10.1 mg		
Appearance:	Lyophilized powder		

SAMPLE PHOTOGRAPH

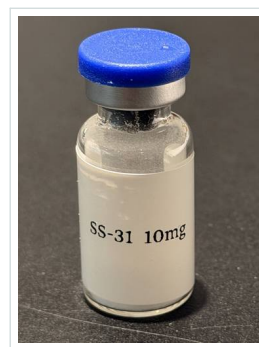

§ 02 Endotoxin Analysis

KINETIC CHROMOGENIC LAL/TAL ENDOTOXIN TEST (USP <85>)

BACTERIAL ENDOTOXIN · KINETIC CHROMOGENIC (QUANTITATIVE)



**below 0.12
EU/mL**

Measured endotoxin below 0.12 EU/mL is **within** the 1 EU/mL limit.

Test method	Kinetic Chromogenic LAL/TAL Endotoxin Test (USP <85>)
Measured endotoxin	below 0.12 EU/mL
Endotoxin limit	1 EU/mL

The endotoxin limit is established by the endotoxin test kit manufacturer.

DISCLAIMER · RESEARCH USE ONLY

Results relate **only to the sample as received** by Side-Chain Analytics Inc. and the tests performed, as and when received — not to any other unit, vial, lot, or batch, and not to any other product bearing the same name, label, or description. This report is not a verification of any lot or batch. **For research use only:** this report is not a certificate of quality, safety, efficacy, or regulatory compliance; the material tested is not authorized by Health Canada for human or veterinary use; and this report is not for human or veterinary administration, clinical or diagnostic use, or label claims. Side-Chain Analytics Inc. does not manufacture, source, or sell the material tested and makes **no warranty, express or implied**; its liability shall not exceed the testing fee. This report may not be reproduced except in full, and may not be reproduced, displayed, quoted, or referenced — in whole or in part, including by any badge, seal, or link — in connection with the advertising, offer for sale, sale, or distribution of any product. This certificate is valid only as currently shown at sidechainanalytics.com/verify and may be withdrawn.