



Preprocessing pipeline


raw HU

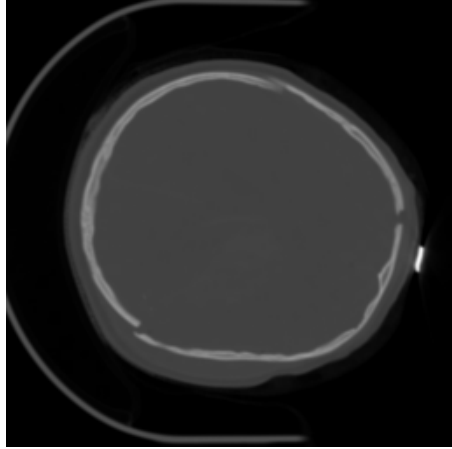


brain window
(40/80)

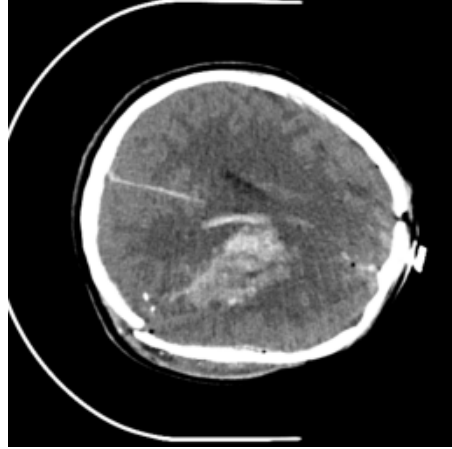


channel 1
(brain + CLAHE)

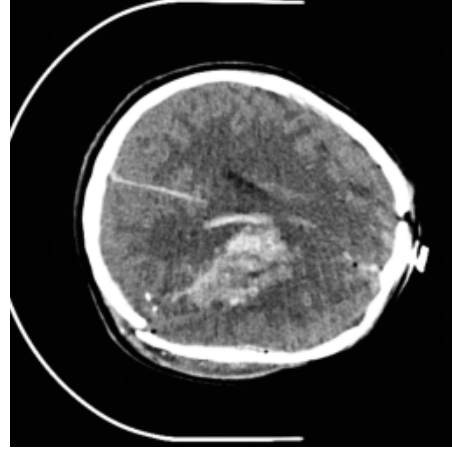


channel 2
subdural (80/200)

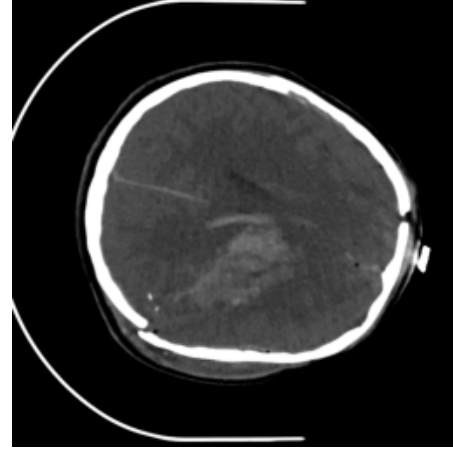

channel 3
bone (600/2800)

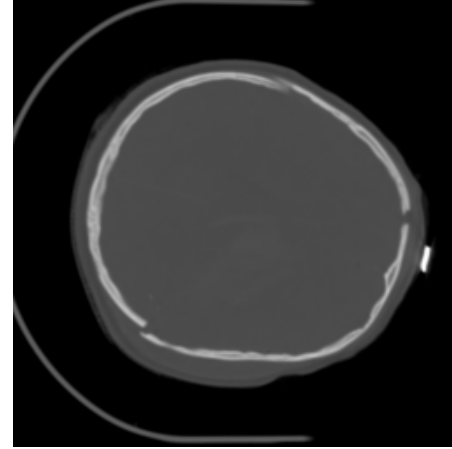

3-window input

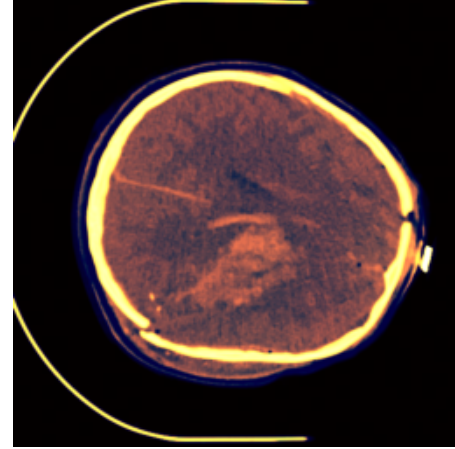

skull strip
(ablation only)

