



Brightness / contrast — +/-12 %, mimicking scanner and reconstruction differences that change apparent blood density


original

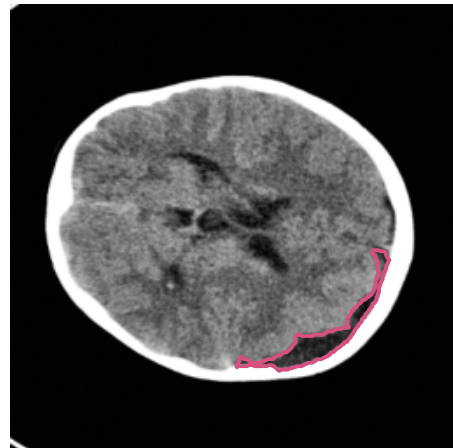


sample 1

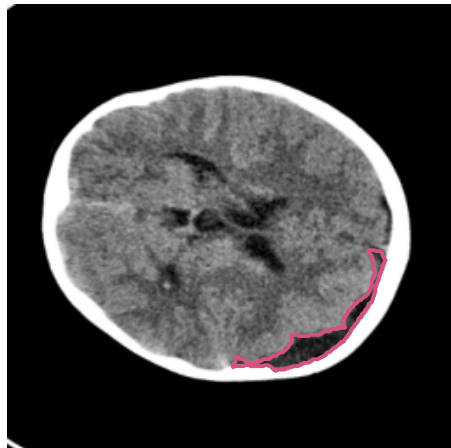

sample 2

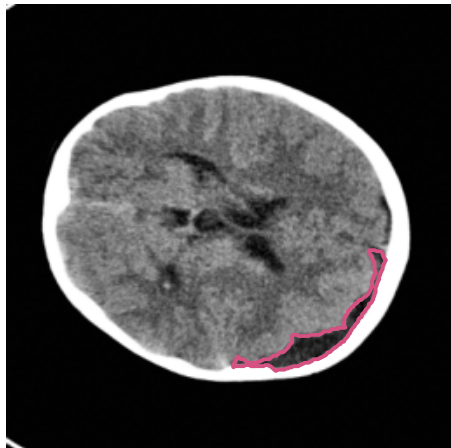

sample 3

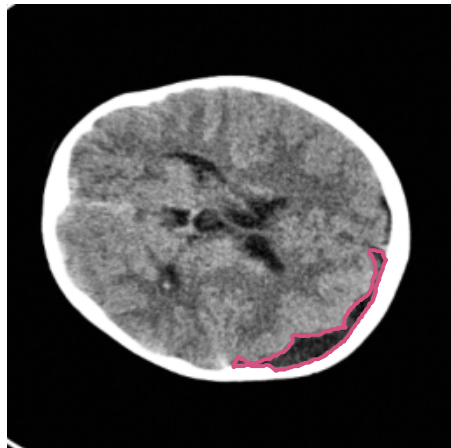

sample 4

