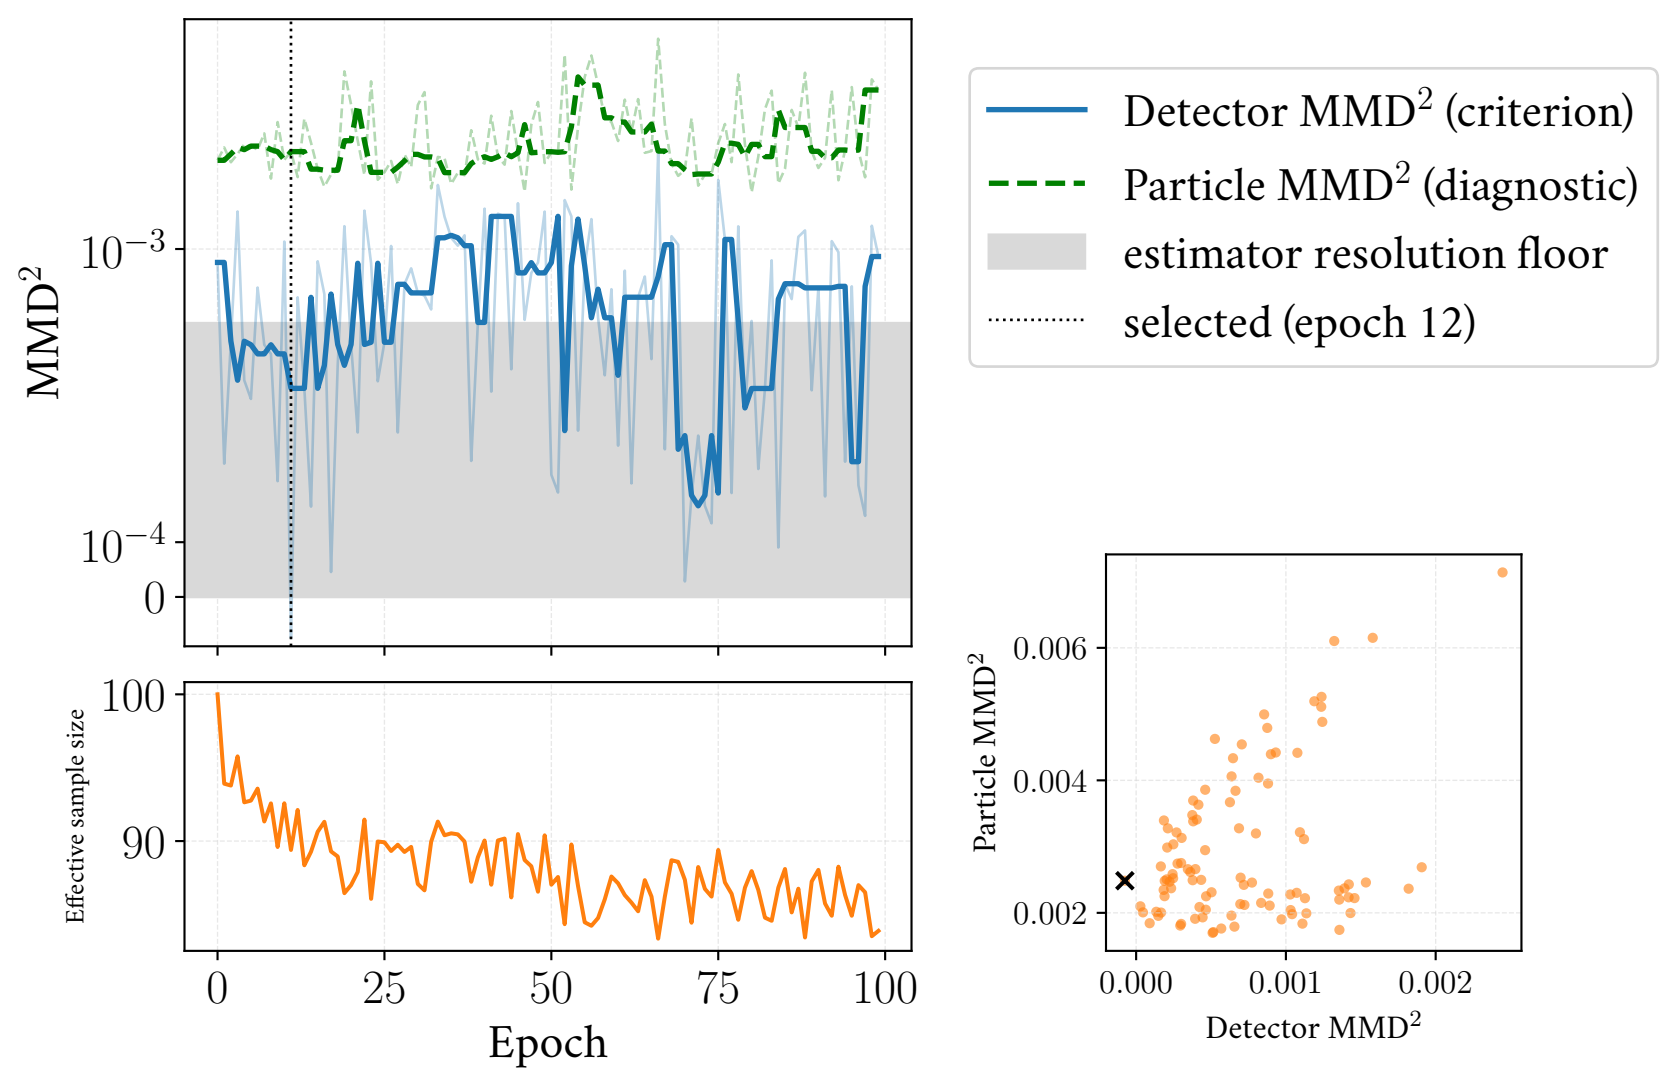

Detector MMD² (criterion)
Particle MMD² (diagnostic)
estimator resolution floor
selected (epoch 12)
MMD²
10⁻³
10⁻⁴
0
Effective sample size
100
90
0
25
50
75
100
Epoch
Particle MMD²
0.006
0.004
0.002
0.000
0.001
0.002
Detector MMD²