Climbing assay: recording setup

None of this is enforced by the software — it analyses whatever it is given and reports how reliable the result is. Following it raises the fraction of recordings that can be scored at all: in the first laboratory set, about half could not be. A protocol improves the INPUT; it does not validate the OUTPUT, which needs counts from a person to compare against.

A Bench arrangement (side view)

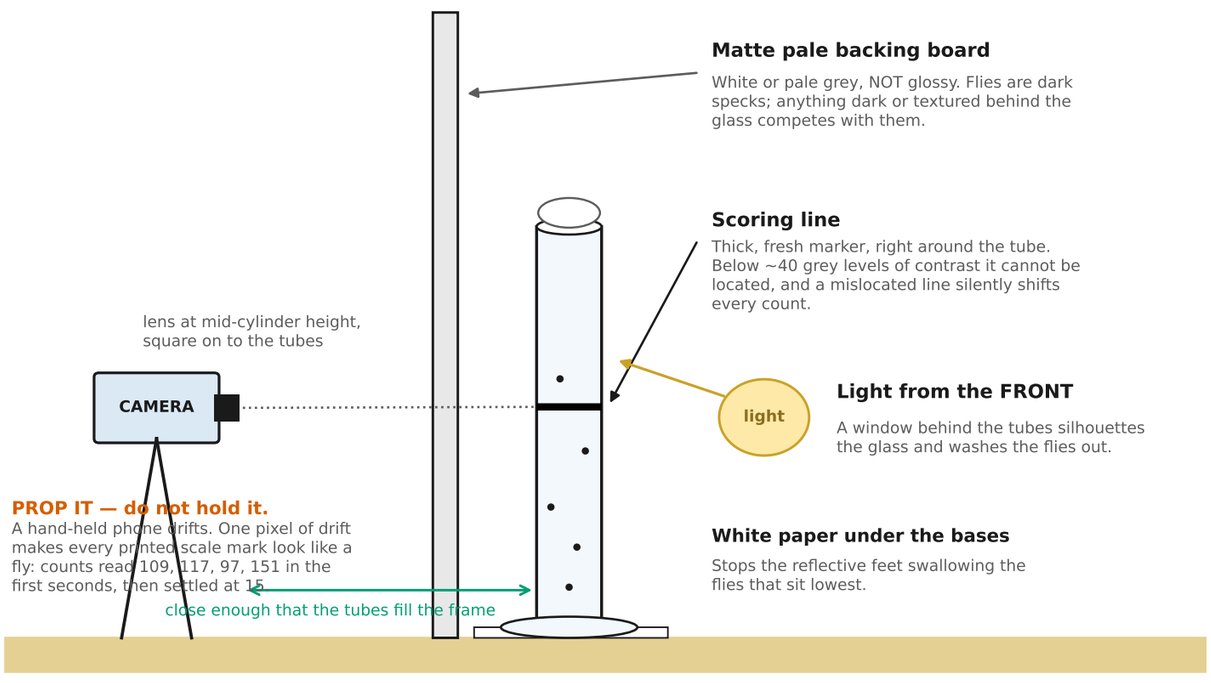

B What you should see before pressing record

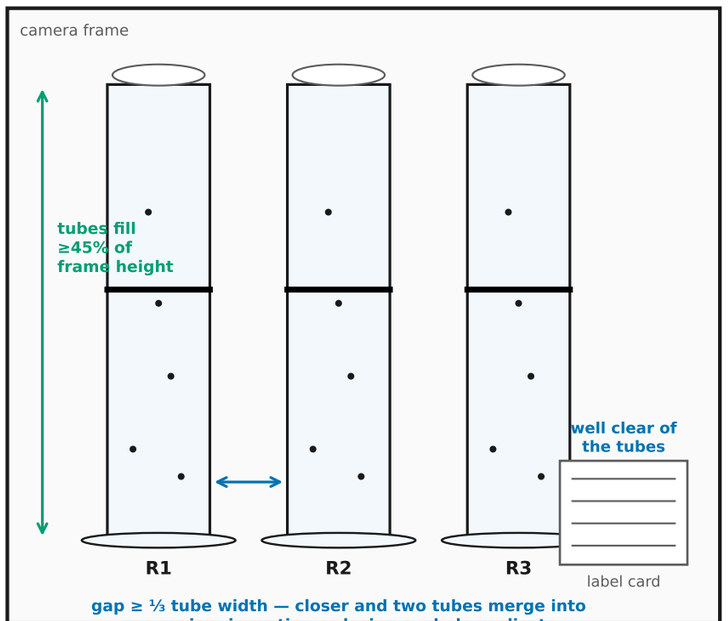

BEFORE YOU PRESS RECORD

- ☐ Phone propped, not held
- ☐ Recording started BEFORE the tap
- ☐ Hands out after the tap
- ☐ Nothing dark behind the tubes
- ☐ Line dark, unbroken, on every tube
- ☐ Flies-per-tube written down
- ☐ Tube diameter noted (25 mm)
- ☐ Each group in ≥2 tubes, ≥2 sessions

THEN CHECK IT

`drophenix_cli.py setup-check test.mov`

Record 30 s of test footage and run that. It measures camera drift, tube spacing, line contrast and framing, and names what to change. Five minutes here saves a session that would otherwise be discarded.