




## A calibration works on the core

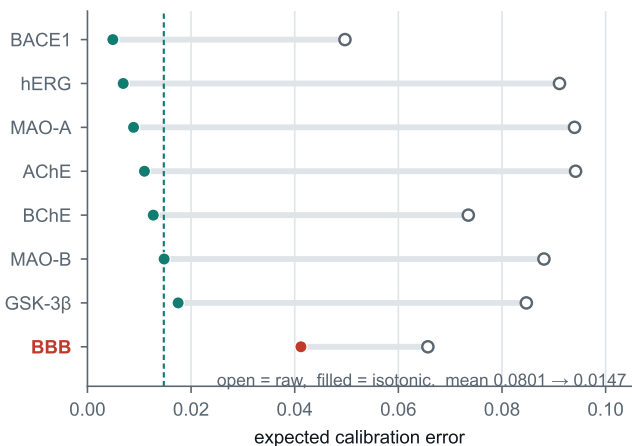

## B and the gate is the worst of them

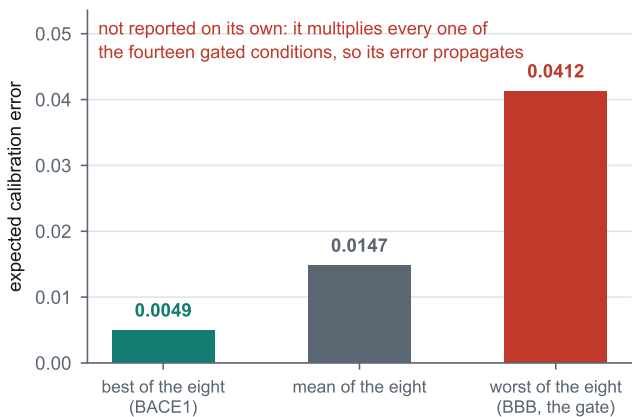

## C conformal coverage, two endpoints short

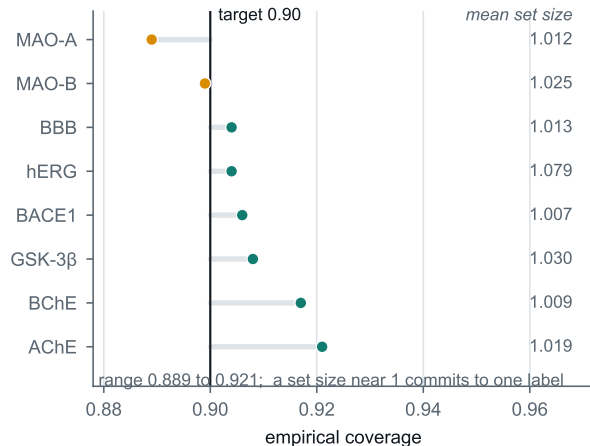

## D where each layer stops

|                                | 8 core classifiers | 47 binder endpoints | 11 ADME, auxiliary |
|--------------------------------|--------------------|---------------------|--------------------|
| isotonic calibration           | 8 of 8             | none                | none               |
| conformal set                  | 8 of 8             | none                | none               |
| applicability band             | 8 of 8             | 39 of 47            | 1 of 11            |
| per-endpoint calibration error | 8 of 8             | 38 of 47            | none               |

Binder calibration error, over the 38 that carry one: mean 0.0762, median 0.0675, range 0.0300 to 0.1780, against 0.0147 for the core. The remaining 9 carry none: CGRP, GABA-A, GBA1, GluN2B, KEAP1, Nav1.5, Nav1.8, SIRT1, α3β4 nAChR