




A calibration works on the core

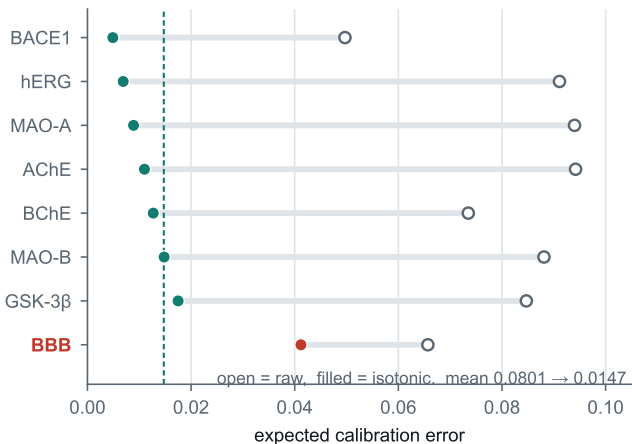

B and the gate is the worst of them

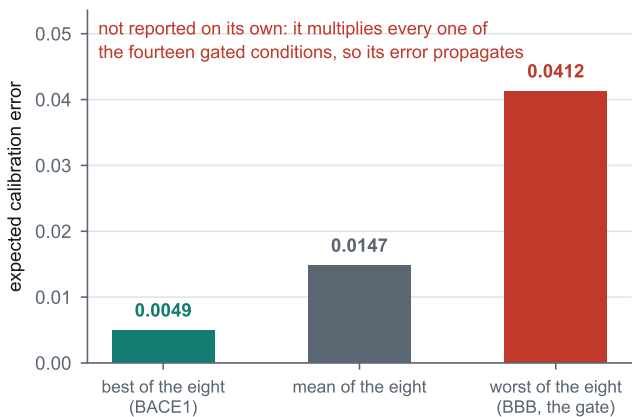

C conformal coverage, two endpoints short

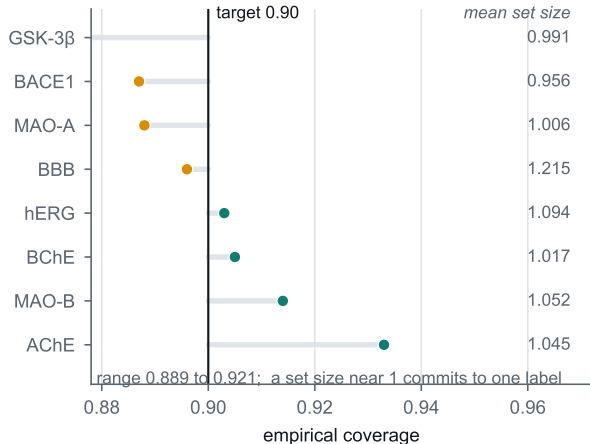

D where each layer stops

	8 core classifiers	47 binder endpoints	11 ADME, auxiliary
isotonic calibration	8 of 8	none	none
conformal set	8 of 8	none	none
applicability band	8 of 8	39 of 47	1 of 11
per-endpoint calibration error	8 of 8	38 of 47	none

Binder calibration error, over the 38 that carry one: mean 0.0762, median 0.0675, range 0.0300 to 0.1780, against 0.0147 for the core. The remaining 9 carry none: CGRP, GABA-A, GBA1, GluN2B, KEAP1, Nav1.5, Nav1.8, SIRT1, α3β4 nAChR