


Threshold Calibration — Fixed $\tau=0.82$ is Not Portable

Calibrated threshold by density bucket



FPR of 0.82 by density bucket (t5)

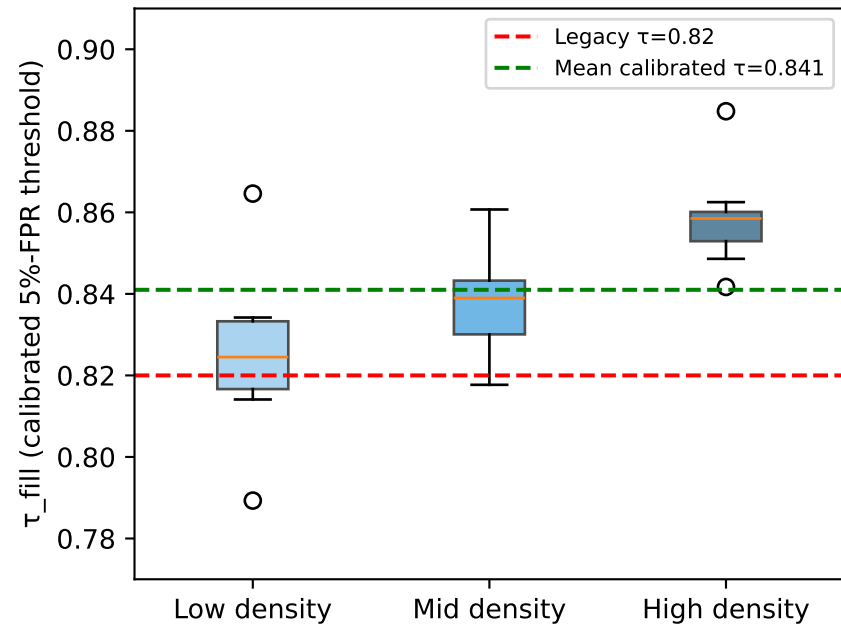