

GR&R; Study Report

Gauge Repeatability & Reproducibility Analysis

Study Date:

2026-05-27

Equipment ID:

O1

Characteristic:

grr_analysis

Method:

Xbar-R

Operators:

N/A

Parts:

N/A

Trials:

N/A

Generated By:

Arad Quality Agent

Component	Value	% Contribution
Repeatability (EV)	0.0124	20.5%
Reproducibility (AV)	0.0566	93.6%
Part Variation (PV)	0.0172	28.5%
Total Variation (TV)	0.0604	100%
GR&R %	95.87%	—
NDC	0	—


NOT ACCEPTABLE

%GR&R; = 95.9% — not_acceptable

NDC = 0

Equipment: O1

Variance Component Breakdown

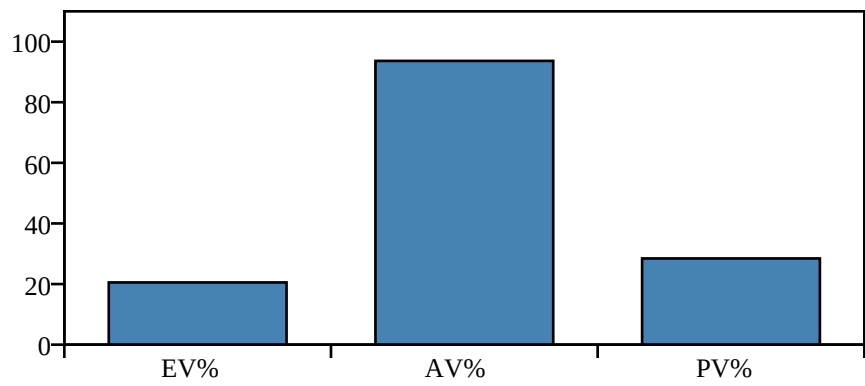

AIAG MSA Reference Guidelines

Threshold	Verdict	Guideline
< 10%	Acceptable	Suitable for production
10-30%	Conditional	Engineering review required
> 30%	Not Acceptable	Must improve before use
NDC ≥ 5	Adequate	Can distinguish parts