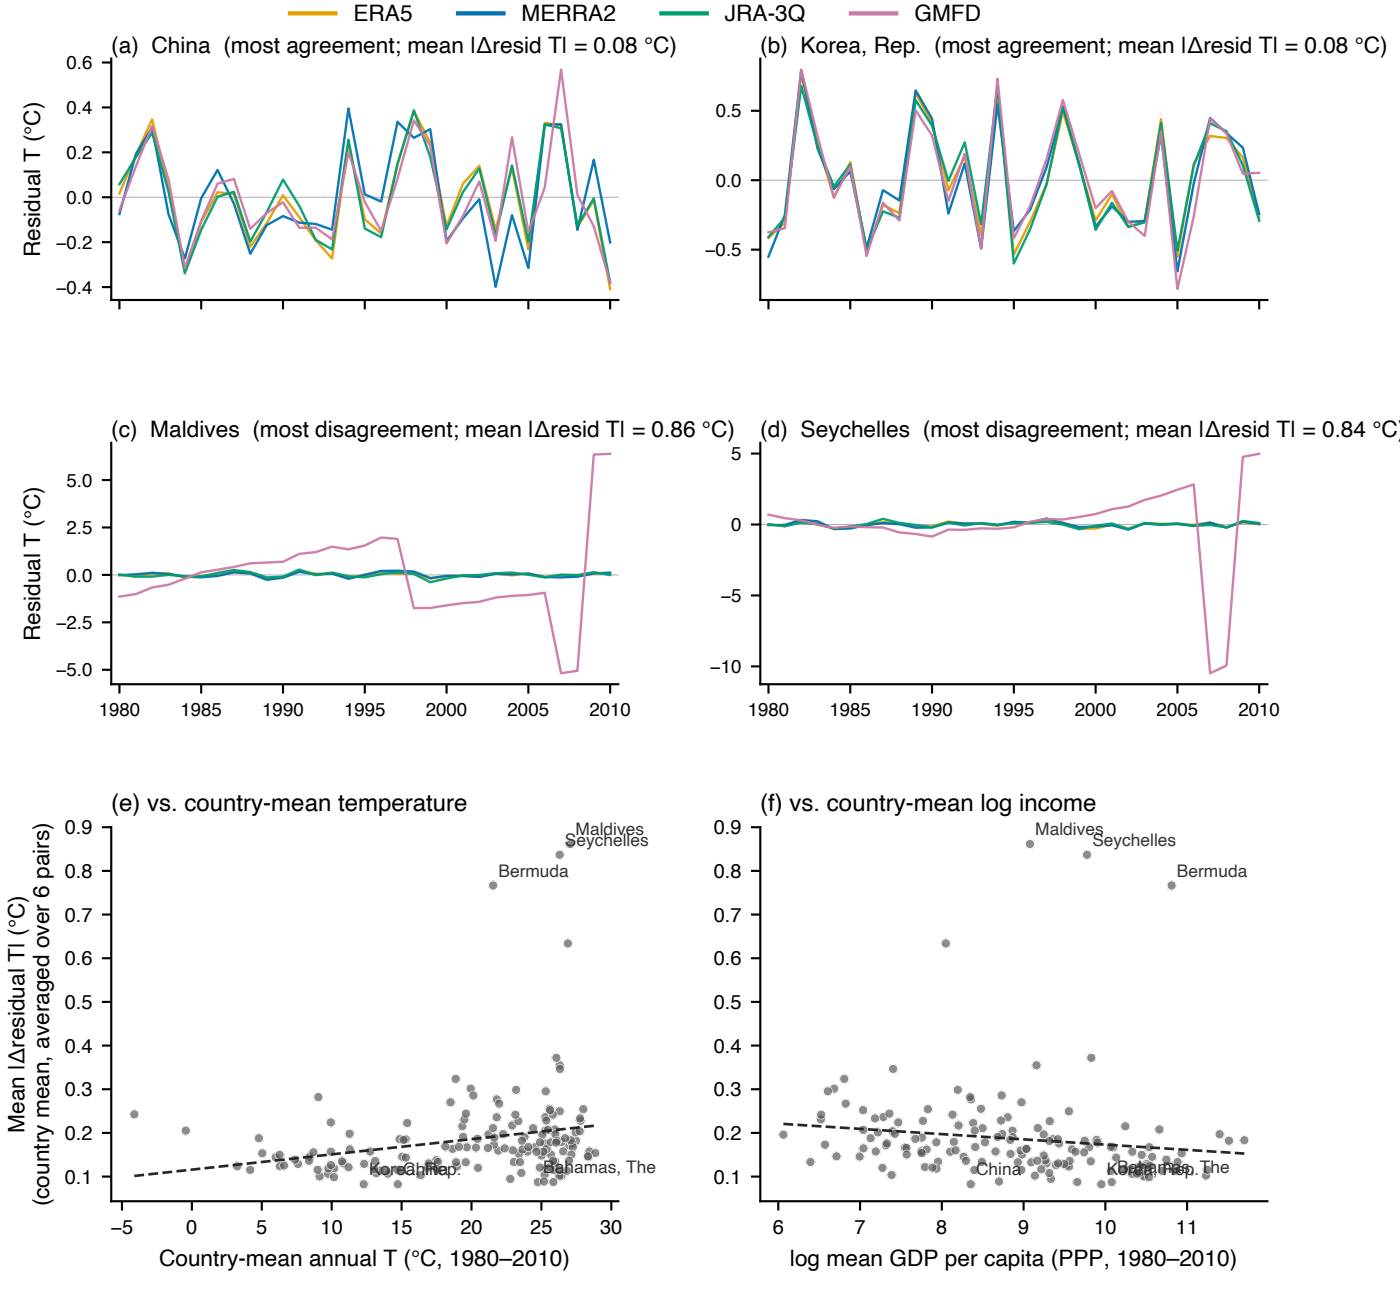Extended Data Fig. 1 Inter-reanalysis disagreement in temperature shocks used to fit the BHM dose-response