


Autotune - 5977C

Tune timestamp: 9/23/2026 4:14 PM (UTC-04:00)

GCMS

D:\MASSHUNTER\GCMS\1\5977\atune_hot300C.u

US2322MA27

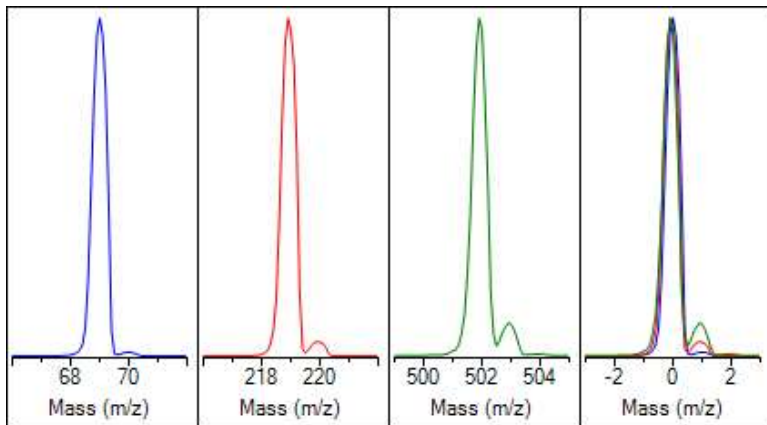


Ion Polarity	Pos	PFTBA	Open
Emission	34.6	Mass Gain	203
Electron Energy	70.0	Mass Offset	-24
Filament	1	Amu Gain	3050
Repeller	32.91	Amu Offset	135.94
Ion Focus	90.3	Width219	-0.032
Entrance Lens	17.6	DC Polarity	Pos
Ent Lens Offset	12.36	HED Enable	On
Ion Body	0.00	EM Volts	2033.0
Post Extractor 1	0	Extractor Lens	0.00
Post Extractor 2	0	Scan Speed	3
JetClean Flow	0.00	Averages	3
Actual/[Setpoint]	[0.00]		

Actual m/z	Abund	Rel Abund	Pw50
69.00	401,375	100.0%	0.59
218.90	329,402	82.1%	0.59
501.90	17,610	4.4%	0.58

Temperatures and Pressures			
MS Source	300	Turbo Speed	100.0
MS Quad	150	Hi Vac	1.18e-05

Low	High	Step	Speed	Threshold	Peaks	Base	Abundance	Total Ion
10.00	701.00	0.10	3	100	109	69.00	390,912	1,361,597

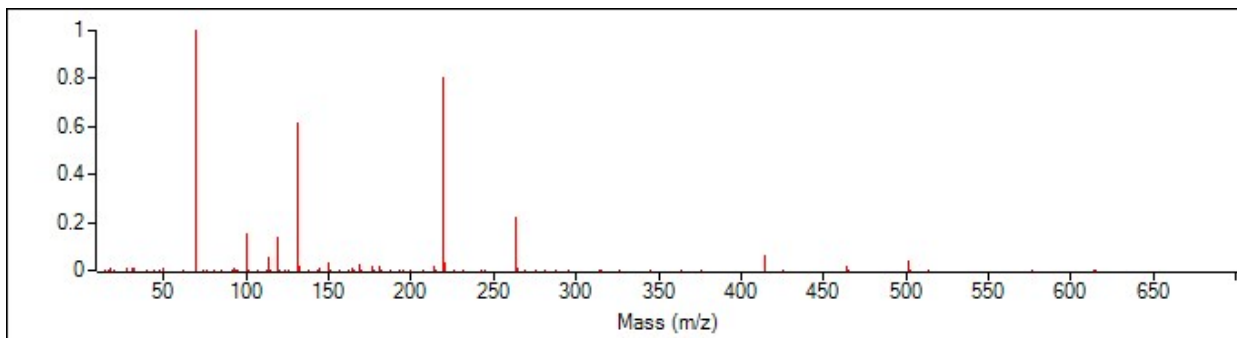

Target m/z	Actual m/z	Abund	Rel Abund	Iso m/z	Iso Abund	Iso Ratio
69.00	69.00	390,912	100.0%	70.00	4,278	1.1%
219.00	219.00	315,136	80.6%	220.00	13,670	4.3%
502.00	502.00	16,760	4.3%	503.00	1,572	9.4%

Air/Water Check: H2O ~0.8% N2 ~1.4% O2 ~0.4% CO2 ~0.2% N2/H2O ~176.6%

Column(1) Flow: 1.10 Column(2): 0.00 ml/min Interface Temp: 320

Ramp Criteria:

Ion Focus maximum 90 volts using ion 502; Electron Multiplier Gain 55883.792

Repeller maximum 35 volts using ion 219; Gain Factor 0.5588

Mass Gain Values(Scan Speed): 212(3) 219(2) 240(1) 258(0) 310(FS1) 336(FS2)

TARGET MASS:	50	69	131	219	414	502	1091
Amu Offset	135.9	135.9	135.9	135.9	135.9	135.9	135.9
Entrance Lens Offset	12.4	12.4	12.4	12.4	12.4	12.4	12.4

Report Created: 9/23/2026 4:14 PM (UTC-04:00)