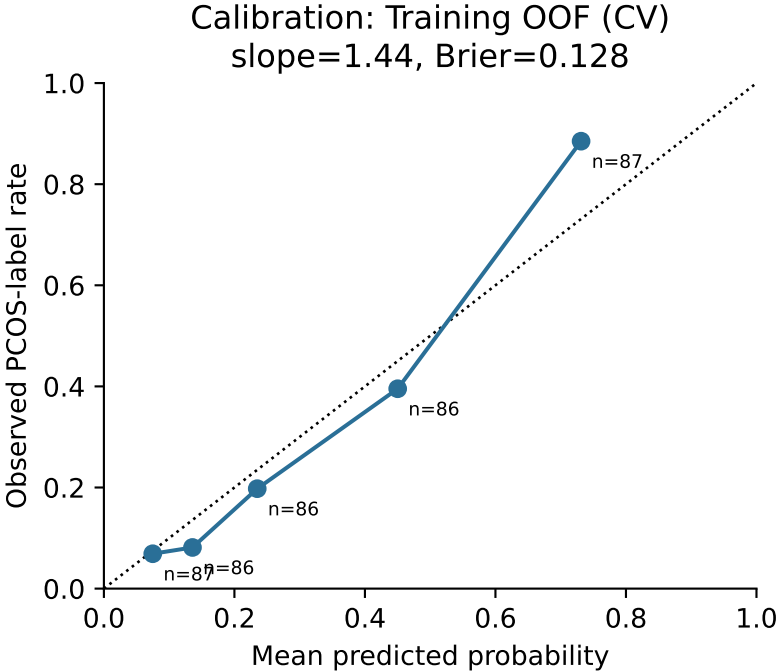
Calibration: Training OOF (CV)
slope=1.44, Brier=0.128
Observed PCOS-label rate
Mean predicted probability
0.0
0.2
0.4
0.6
0.8
1.0
n=87
n=86
n=86
n=86
n=87

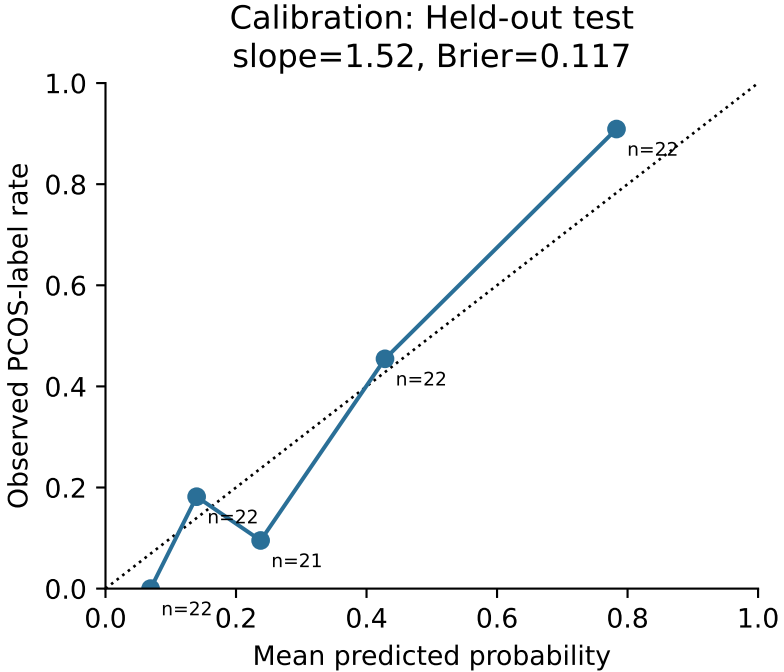
Calibration: Held-out test
slope=1.52, Brier=0.117
Observed PCOS-label rate
Mean predicted probability
0.0
0.2
0.4
0.6
0.8
1.0
n=22
n=22
n=22
n=21
n=22