

CALIBRATION

CERTIFICATE



LionTu
INSTRUMENTATION

Customer	: ABC Manufacturing Ltd 123 Industrial Road Harare South Africa
Instrument	: Digital Weight Scale
Make/ Model	: Mettler Toledo PB 3002-S
Range	: N/A
Serial Number	: METTLER-SN-2024-0001
Control No	: LAB-SCALE-001
Location	: Lab Building A, Room 102
Date of calibration	: 25 May 2026
Calibration due date	: 25 May 2027
Temperature	: 25°C ± 2 °C
Humidity	: 50% ± 10%


Standard/Reference Details.

Instrument	Manufacturer	Serial Number
MASS PIECES	LTI	LT-MP (
STANDARD MASS WEIGHTS	LTI	-



VERIFY ONLINE

The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k=2$ providing a level of confidence of approximately 95%, the uncertainty of measurement has been estimated in accordance with the BIPM, IEC, ISO, IUPAP, OIML document principles defined in the GUM, Guide to Uncertainty of Measurement, ISO, Geneva, 1993'. The correct reading is obtained by adding the correction to the reading on the unit under test. The measurement result is related only to the calibrated unit. The calibration certificate or report may not be reproduced except in full, without the written approval of the laboratory.

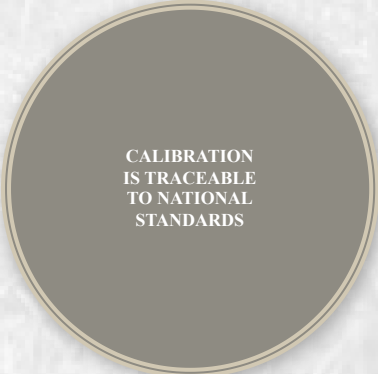

allone

Calibrated by: [\(GT. CHAPANANGA\)](#)

CALIBRATION AND SERVICE REPORT

Table of Instrument readings Certificate No: CERT-2026-00001 compared with those of standard mass weights.

TABLE OF RESULTS:

STANDARD (KG)	UUT POST-CAL (KG)	CORRECTION (KG)
---------------	-------------------	-----------------

CALIBRATION SUMMARY:

Procedure: Calibrated according to standard LionTurf procedures.

Traceability: ISO 17025:2017

Comment: All measurements within SAZ tolerance limits.

Note : The measurement results recorded in this certificate were correct at the time of calibration. The subsequent accuracy will depend on factors such as care, handling and frequency of use. If used properly next check is recommended in August 2026

S. Chidzvondo

Calibrated by: (S. Chidzvondo)