


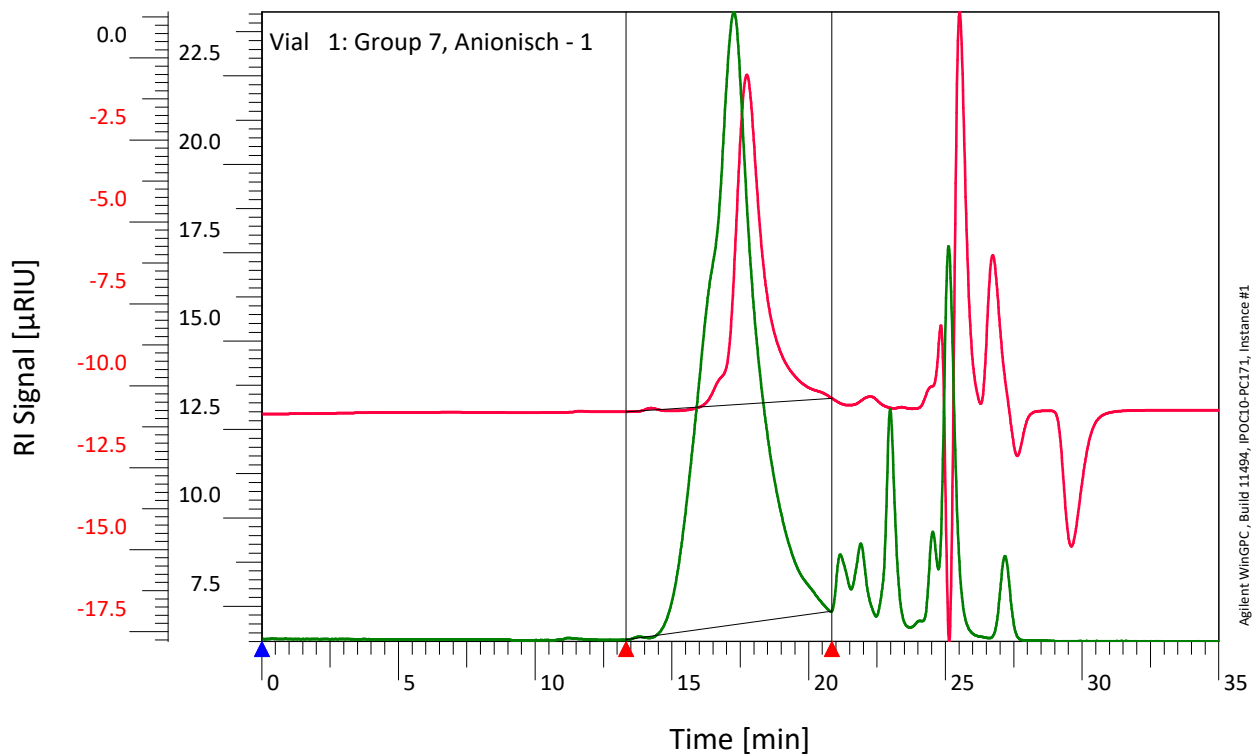

Sample : Vial 1: Group 7, Anionisch - 1
Baseline from : 13.322 ml
Integration from : 14.532 ml
Calibration File : \PS-THF-50ul-PW...2026_big columns.CAL
MHK - A (Cal.): 0.000E+0
Int.stand.-cal.: 50.000 ml
Pump : Agilent G7110B
Concentration : 1.000 g/l
Column 1 : PSS SDV
Column 2 : PSS SDV
Column 3 : PSS SDV
Detector 1 : I1: RID 1, RI Signal
Detector 2 : I1: VWD 1, Signal A
Detector 3 : I1: IsoPump 1, Pressure
Operator : local_admin

Method : GPC1.MET
to : 20.851 ml
to : 20.591 ml
Eluent : THF
MHK - K (Cal.): 1.000E+0 ml/g
Int.stand.-sam.: ----- ml
Flowrate : 1.000 ml/min
Inject volume : 100.000 ul
Temperature : 0.000 °C
Temperature : 0.000 °C
Temperature : 0.000 °C
Delay volume : 0.000 ml
Delay volume : 0.000 ml
Delay volume : 0.000 ml
Acquisition interval : 1.000 sec