DXCONNECTION

Calibration Services Division

Valley Precision Instrument Calibration Services
1187 N. Willow Ave. Suite 103, Clovis, CA 93611
Ph: 1+ (559) 260-5511 Fax: 1+ (559) 260-5512

CERTIFICATE OF CALIBRATION

Prepared for:
Lee Bussy
1237 Eagle
Hillsboro KS 67063-8071
United States

Certificate No: DXC-2026-3339-002

INSTRUMENT INFORMATION

Inst. Description: Power Sensor
Manufacturer: Agilent
Model: 8482A
Serial Number: MY41094127
Cust. ID. No.: N/A
Accuracy: MM

Calibration Site: In Shop
Date Received: N/A
Date of Cal.: 15 Oct 2026
Next Cal. Due: 15 Oct 2027
Proc.: MM
Calibration Result: Passed

as Received	As Left
	In Tolerance
Operational	Operational
	Full Calibration

STANDARDS USED

Model No.	Manufacturer	Description	Cal Date Due Date	Uncertainty
83712A	Agilent	Microwave Sig Gen	14-Jun-2027	+/- 1.6%
11667A	Agilent	Power Splitter	17-Jan-2027	+/- 0.35%
E4419B	Agilent	Power Meter	24-Apr-2027	+/- 1.3%
8753ES	Agilent	Network Analyzer	31-Jul-2027	+/- 1.2%
85032F	Agilent	Calibration Kit	21-Oct-2027	+/- 1.0°
N8481D CFT	Agilent	Average Power Sensor	28-Feb-2027	+/- 1.3%

TEST ROOM ENVIRONMENT

Temperature: 22.0C / 71.6 F Relative Humidity: 23.6% Barometric Pressure: N/A in. Hg

V P I C S certifies that the above listed instrument meets or exceeds all published specifications. It has been calibrated using standards whose accuracies are traceable to the National Institute of Standards and Technology. Alternatively, accuracy has been derived from accepted values of natural physical constants or have been derived by the ratio type of self-calibration techniques. This certificate may be reproduced in full. Partial reproduction may be done only with written prior consent of V P I C S. Calibration is performed using procedures and standards traceable to the National Institute of Standards

Measurements certified by: David R. Smith ***Date:*** 10/15/2026


Title: Sr Eng

Agilent

8482A Power Sensor

Calibration Chart

MY41094127	C.F. 99%	15-Oct-2026
Frequency	EE%	Cal Fact
MHz.	dBm	%
0.1	0.00	100.7
0.3	0.00	100.7
1.0	0.00	100.7
3.0	0.00	100.9
10.0	0.00	101.1
30.0	0.00	100.9
50.0	0.00	99.0
100.0	0.00	100.6
300.0	0.00	99.9
1000.0	0.00	97.0
2000.0	0.00	98.0
3000.0	0.00	93.3
4000.0	0.00	94.0
4200.0	0.00	93.4

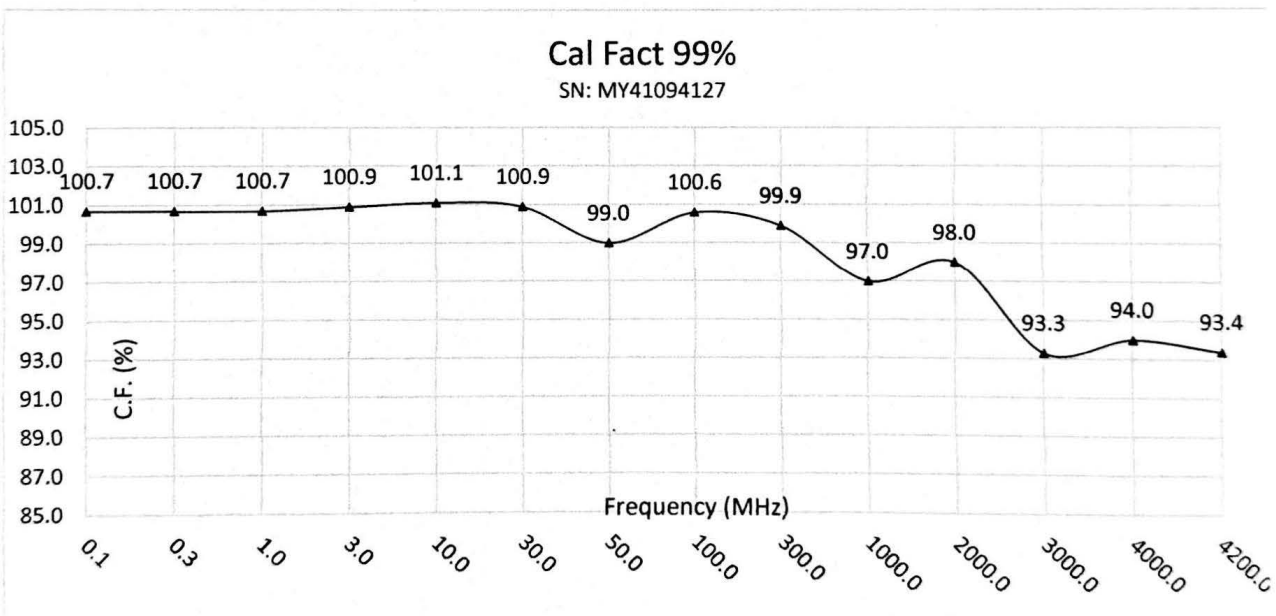

Typical measurement uncertaintities of calibration factor	
100 KHz to 10 MHz	0.87%
10 MHz to 1.2 GHz	0.80%
1.2 GHz to 4.2 GHz	0.90%