SYNTHETIC BIOSENSOR STUDY - SOFTWARE DEMO

This is a generated test document, not a published paper.

No patient samples, real measurements, DOI, or clinical claims are included.

Purpose: demonstrate a biosensor paper-reading workflow.

Recognition element: a hypothetical affinity probe on a sensing surface.

Transduction: simulated fluorescence intensity proportional to concentration.

Methods (all invented for software testing): PBS buffer, room temperature,

15 minute incubation. Concentrations: 0, 1, 2, 4, 8 nM.

Three synthetic replicate values at each concentration; see the CSV fixture.

Control: a simulated blank. Matrix selectivity and stability were not tested.

These conditions are not a validated experimental protocol.

RESULTS AND LIMITATIONS - SYNTHETIC ONLY

Mean signals: 0.04, 0.20, 0.42, 0.79, 1.59 arbitrary units.

Figure 1 illustrates the five synthetic means.

Detection limit and clinical sensitivity were not measured or reported.

There is no real sample validation, specificity study, or stability study.

The document tests page citations and figure reading only.
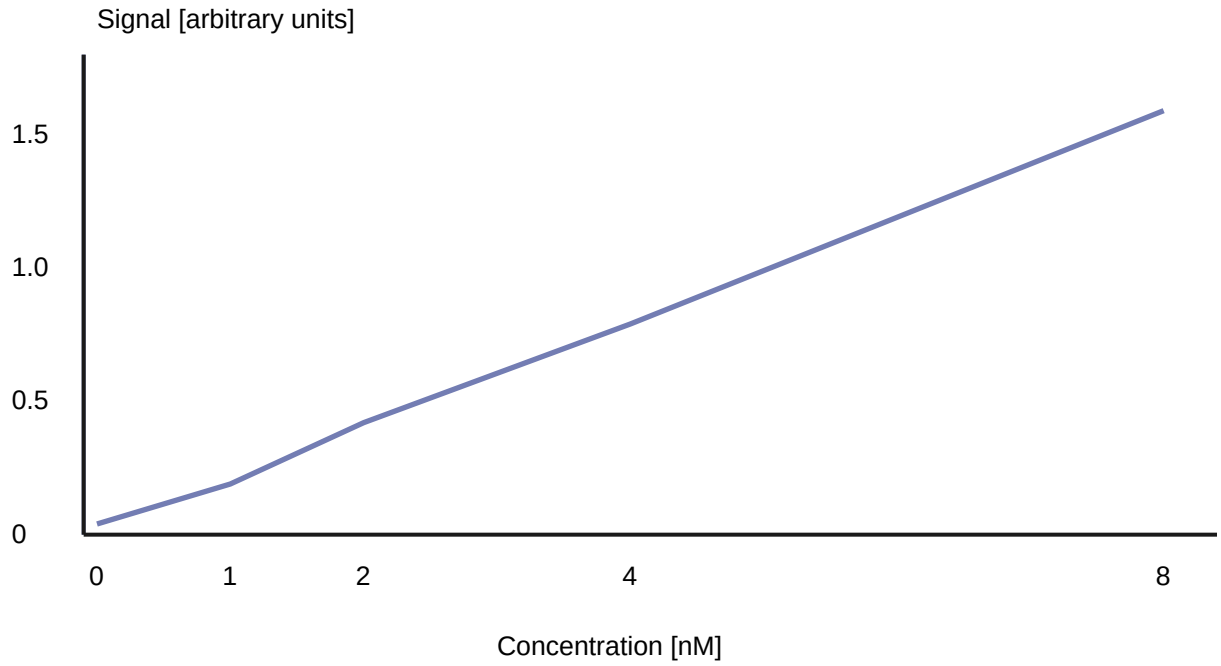
Figure 1. Synthetic calibration means - not experimental evidence.