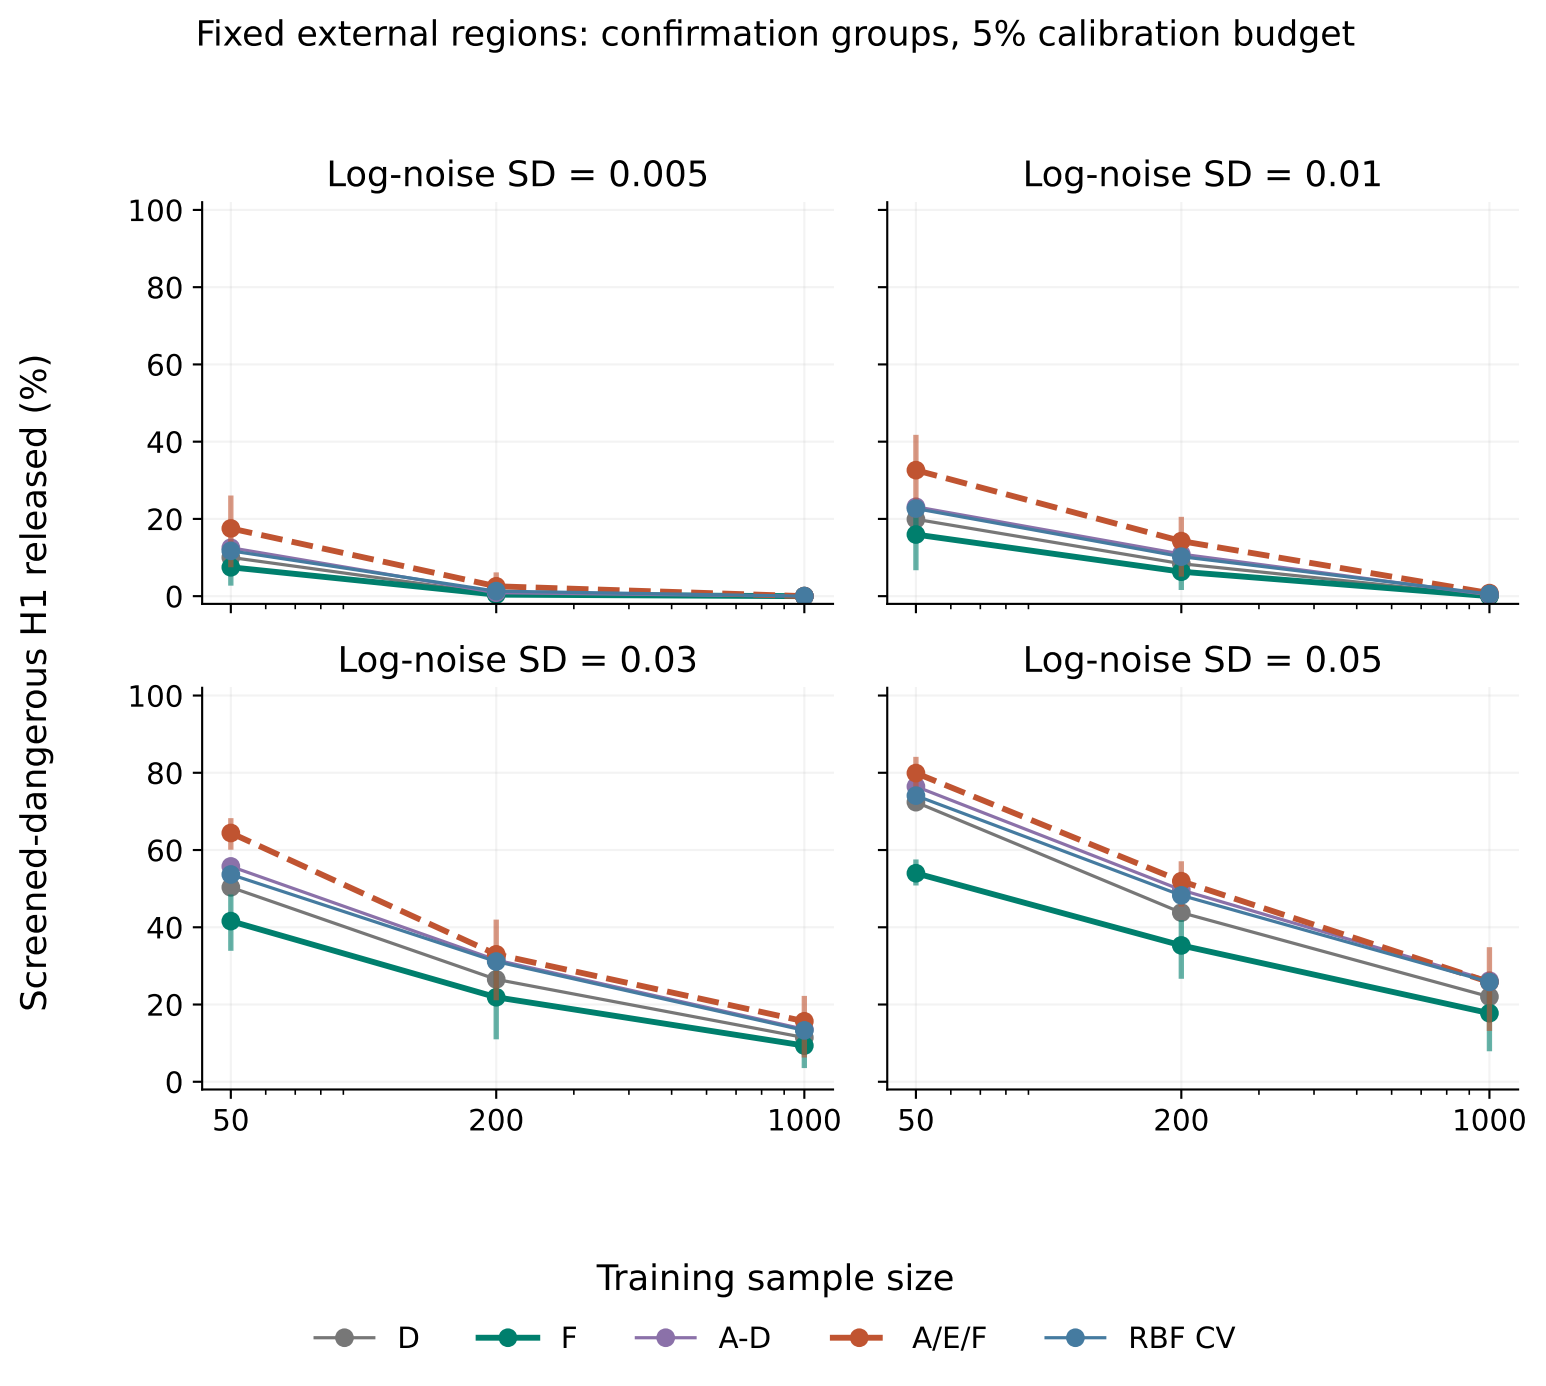
Fixed external regions: confirmation groups, 5% calibration budget
Log-noise SD = 0.005
Log-noise SD = 0.01
Log-noise SD = 0.03
Log-noise SD = 0.05
Screened-dangerous H1 released (%)
0
20
40
60
80
100
50
200
1000
Training sample size
D
F
A-D
A/E/F
RBF CV