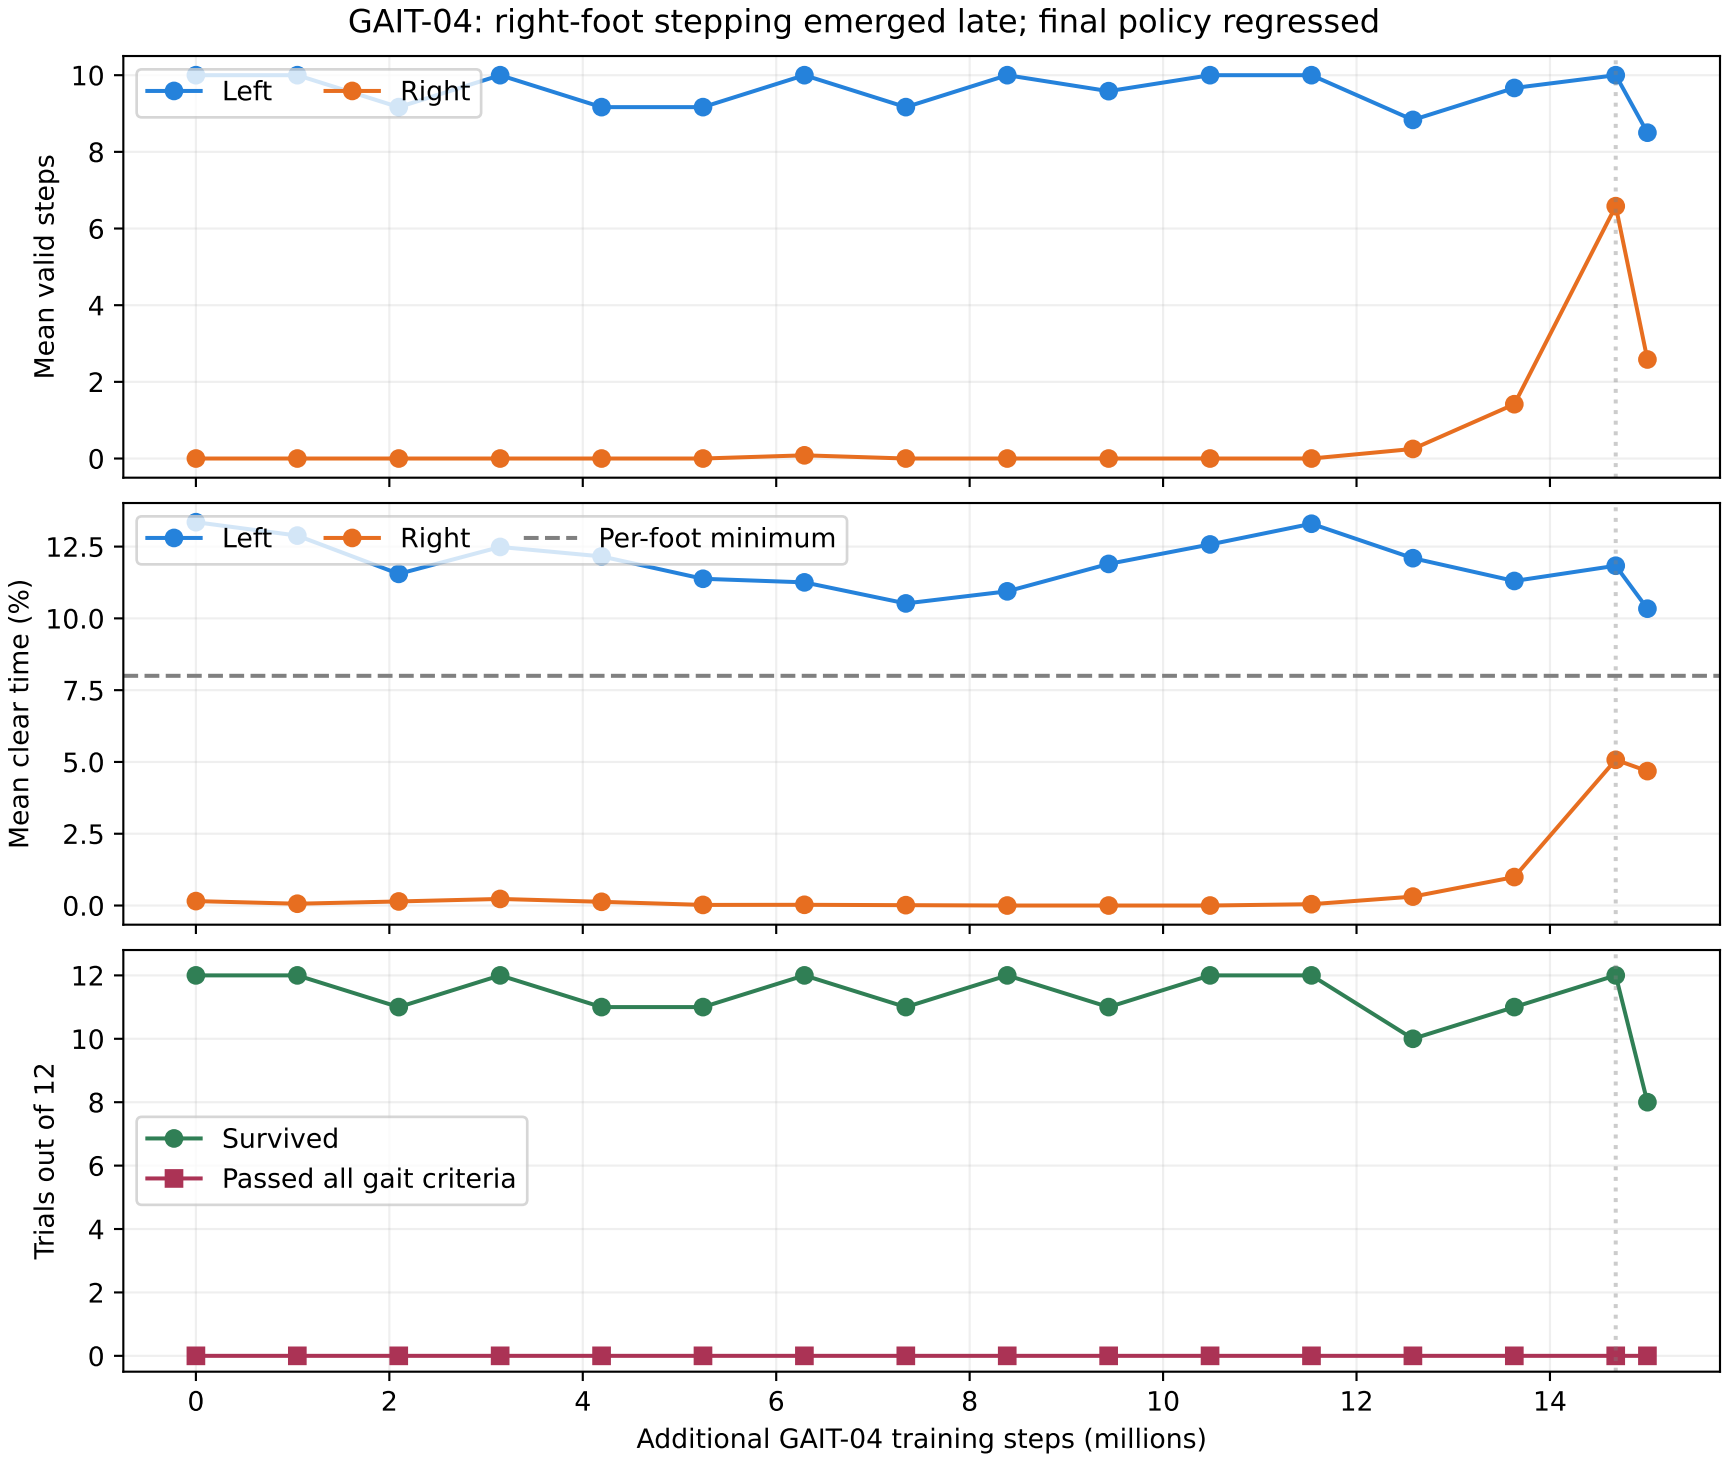
GAIT-04: right-foot stepping emerged late; final policy regressed
Mean valid steps
Left
Right
Mean clear time (%)
Left
Right
Per-foot minimum
Trials out of 12
Survived
Passed all gait criteria
Additional GAIT-04 training steps (millions)
Quality: seconds 5–25 before termination; early falls shorten the window.
Clearance threshold: 1.5 cm. These are evaluation means, not video measurements.