

# Advanced 3D Monte Carlo Algorithms for Biophotonic and Medical Applications

Lewis McMillan



University of  
St Andrews

This thesis is submitted in partial fulfilment for the degree of  
PhD  
at the  
University of St Andrews

March 2019



# Declaration

I, Lewis McMillan, hereby certify that this thesis, which is approximately \*\*\*\*\* words in length, has been written by me, that it is the record of work carried out by me, or principally by myself in collaboration with others as acknowledged, and that it has not been submitted in any previous application for a higher degree.

I was admitted as a research student in September 2015 and as a candidate for the degree of PhD in September 2015; the higher study for which this is a record was carried out in the University of St Andrews between 2015 and 2019.

Date ..... Signature of candidate .....

I hereby certify that the candidate has fulfilled the conditions of the Resolution and Regulations appropriate for the degree of PhD in the University of St Andrews and that the candidate is qualified to submit this thesis in application for that degree.

Date ..... Signature of supervisor .....

Date ..... Signature of supervisor .....



# Abstract

Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum.

Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris.



# Acknowledgements

Lorem ipsum dolor sit amet, consectetur adipiscing elit. Ut purus elit, vestibulum ut, placerat ac, adipiscing vitae, felis. Curabitur dictum gravida mauris. Nam arcu libero, nonummy eget, consectetur id, vulputate a, magna. Donec vehicula augue eu neque. Pellentesque habitant morbi tristique senectus et netus et malesuada fames ac turpis egestas. Mauris ut leo. Cras viverra metus rhoncus sem. Nulla et lectus vestibulum urna fringilla ultrices. Phasellus eu tellus sit amet tortor gravida placerat. Integer sapien est, iaculis in, pretium quis, viverra ac, nunc. Praesent eget sem vel leo ultrices bibendum. Aenean faucibus. Morbi dolor nulla, malesuada eu, pulvinar at, mollis ac, nulla. Curabitur auctor semper nulla. Donec varius orci eget risus. Duis nibh mi, congue eu, accumsan eleifend, sagittis quis, diam. Duis eget orci sit amet orci dignissim rutrum.

Nam dui ligula, fringilla a, euismod sodales, sollicitudin vel, wisi. Morbi auctor lorem non justo. Nam lacus libero, pretium at, lobortis vitae, ultricies et, tellus. Donec aliquet, tortor sed accumsan bibendum, erat ligula aliquet magna, vitae ornare odio metus a mi. Morbi ac orci et nisl hendrerit mollis. Suspendisse ut massa. Cras nec ante. Pellentesque a nulla. Cum sociis natoque penatibus et magnis dis parturient montes, nascetur ridiculus mus. Aliquam tincidunt urna. Nulla ullamcorper vestibulum turpis. Pellentesque cursus luctus mauris.

# Contents

<b>Declaration</b>	<b>iii</b>
<b>Abstract</b>	<b>v</b>
<b>Acknowledgements</b>	<b>vii</b>
<b>Abbreviations</b>	<b>ix</b>
<b>List of Figures</b>	<b>x</b>
<b>1 Introduction</b>	<b>1</b>
1.1 Monte Carlo Method . . . . .	1
1.2 Thesis Outline and Objective . . . . .	4
1.3 Synopsis and Thesis Objectives . . . . .	4



# Abbreviations

**CDF** cumulative distribution function.

**MCRT** Monte Carlo radiation transfer.

**PDF** probability density function.

# List of Figures

- 1.1 Sample Buffon needle experiment. 100 needles are dropped on a  $10 \times 10$  cm area with lines spaced 1.5 cm apart. If a needle lands on a line it is recorded and coloured blue, else it is red. This simulation gave a value of  $\pi \approx 3.10$ .
- 1.2 Illustration of the rejection method for determining  $\pi$  from the area of a circle inscribed within a square. The ratio of the area of the circle to the square is  $\frac{\pi}{4}$ . Thus the ratio of darts landing in the circle to those that land outside the circle is  $\pi \approx \frac{4N_{inner}}{N_{total}}$ , where  $N_{total}$  is the total number of darts, and  $N_{inner}$  is the total number of darts that land in the circle. Using 200 darts gave a value of  $\pi \approx 3.12$ .
- 1.3 Example of randomly sampling from a spectrum. Figure shows 100 random samples drawn to recreate a solar spectrum.
- 1.4 Computer generated imagery using ray tracing. The Monte Carlo method is used to “compute radiance along ray paths between lights and the camera”, to generate CGI images [16].

# Chapter 1

## Introduction

Medical knowledge in the last century has come on leaps and bounds. One particular area of research is into so called “digital twin”. A digital twin as defined by A El Saddik [1]:

“A digital twin is a digital replica of a living or non-living physical entity.”

allow tests on digital counterpart, no need for invasive, painful or tests that may have adverse affects. Saves from animal testing too. mention nasa apollo 13 used in industry - example philips mri machine. used to keep track of equipment, id maintenance before they arise etc parlay this into humans, and thus mcr speak about mcr a wee bit then link onto next paragraph

srcs: <https://www.philips.com/a-w/about/news/archive/blogs/innovation-matters/20180830-the-rise-of-the-digital-twin-how-healthcare-can-benefit.html>

### 1.1 Monte Carlo Method

The Monte Carlo method is a numerical analysis technique based upon random numbers, which are used to calculate unknown variables in problems [2, 3].

The earliest use of the method is in Buffon’s needle experiment of the 18<sup>th</sup> century [4-6]. Buffon asked the question;


“Suppose we have a floor made of parallel strips of wood, each the same width, and we drop a needle onto the floor. What is the probability that the needle will lie across a line between two strips?”

The solution to this question is: for a needle length  $l$ , strip separation  $s$ , where  $x$  is the distance from the needle to the closest line, and  $\theta$  is the angle of the needle with respect to the wood strips. Then using a simple geometrical argument, a needle crosses a strip if  $x \leq \frac{l}{2} \sin \theta$ .

$x$  is distributed uniformly in  $[0, \frac{s}{2}]$ , and  $\theta$  in  $[0, \frac{\pi}{2}]$ . Therefore the probability density function for  $x$  is  $p(x) = \frac{2}{s}$ , and  $\theta$  is  $p(\theta) = \frac{2}{\pi}$ . The probability density function (PDF), is a function of a variable that gives probability for a variable to take a given value. The PDF is normalised over the whole range of the variable, in this case  $x$ , and  $\theta$ . Thus, as  $x$  and  $\theta$  are independent variables, giving a joint probability of  $p(x, \theta) = \frac{4}{s\pi}$ . So the probability of a needle of length  $l$  ( $l < s$ ) is:

$$P = \int_0^{\frac{\pi}{2}} \int_0^{\frac{l}{2} \sin \theta} \frac{4}{s\pi} dx d\theta = \frac{2l}{s\pi} \quad (1.1)$$

Equation (1.1) can be used to carry out a Monte Carlo estimation of  $\pi$ . A simple rearrangement yields:  $\pi = \frac{2l}{sP}$  where  $P$  is the ratio of needles crossing the line to the total number dropped. Laplace was the first to suggest that Buffon's needle experiment could be used to estimate  $\pi$  [5]. Figure 1.1 shows an example of a simulation of Buffon's needle experiment.




**Figure 1.1:** Sample Buffon needle experiment. 100 needles are dropped on a  $10 \times 10$  cm area with lines spaced 1.5 cm apart. If a needle lands on a line it is recorded and coloured blue, else it is red. This simulation gave a value of  $\pi \approx 3.10$ .

There are various different approaches to using the Monte Carlo method to obtain randomly sampled variables. One analytical way of achieving this is the inverted sampling method. The inverted sampling method can be summarised by the following steps for drawing a sample  $X_i$  from an arbitrary PDF  $p(x)$ :

1. Compute the cumulative distribution function (CDF)  $P(x) = \int_0^x p(x')dx'$
2. Compute the inverse  $P^{-1}(x)$
3. Obtain a uniformly distributed random number  $\xi$
4. Finally, compute  $X_i = P^{-1}(\xi)$


If a given problem cannot use the inverted sampling method, as it may not be possible to get a PDF or analytically invert the CDF, then the rejection method can be used. The rejection method is essentially a dart throwing method. This means that points are drawn and compared to the function. If the point lies under the function then the point is accepted, if it lies above the function then it is rejected. For example, if a function,  $f(x)$  that does not have an analytical PDF, we can use a PDF  $p(x)$  such that  $f(x) < cp(x)$  where  $c$  is a constant. Therefore sampling from  $p(x)$ , and if the sampled point lies under  $f(x)$  it is accepted, else it is rejected. Figure 1.2 shows an example of this process.

One common use of the Monte Carlo method, is to randomly sample from a spectrum. To generate a random sample from a spectrum, first the CDF of the spectrum must be calculated. This is done by first normalising the PDF, where the pdf in this case is the spectrum it self. It is normalised such that the sum of the PDF is unity. The CDF is then just the cumulative sum of the PDF. Then using the above method as described above, a random number is drawn,  $\xi$ ,



**Figure 1.2:** Illustration of the rejection method for determining  $\pi$  from the area of a circle inscribed within a square. The ratio of the area of the circle to the square is  $\frac{\pi}{4}$ . Thus the ratio of darts landing in the circle to those that land outside the circle is  $\pi \approx \frac{4N_{\text{inner}}}{N_{\text{total}}}$ , where  $N_{\text{total}}$  is the total number of darts, and  $N_{\text{inner}}$  is the total number of darts that land in the circle. Using 200 darts gave a value of  $\pi \approx 3.12$


and the bracketing values in the CDF are found. We then interpolate to get the x and y values corresponding to  $\xi$ . Figure 1.3

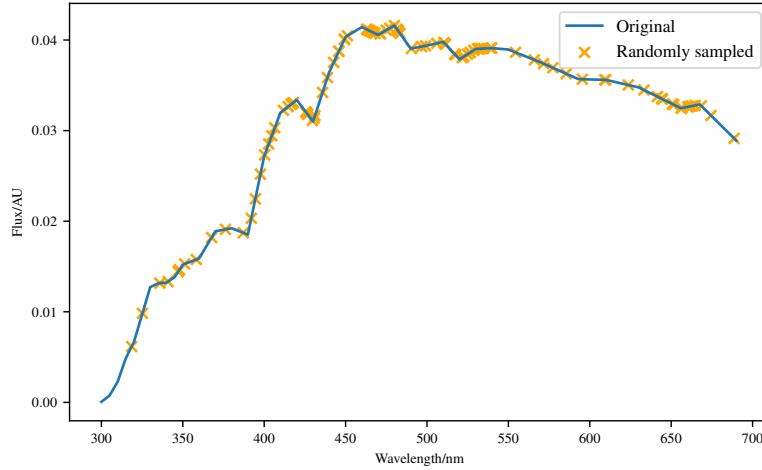

**Figure 1.3:** Example of randomly sampling from a spectrum. Figure shows 100 random samples drawn to recreate a solar spectrum.

The Monte Carlo method is used in various different disciplines. Ranging from use in the financial sector to analyse investments and stocks by simulating the sources of uncertainty which affect their values [7,8], use in statistical analysis [9], and in modern computer generated images (see Fig. 1.4) [10,11]. It is also widely used in astronomy [12,13] and medicine [14,15], to simulate the propagation of radiation through scattering (turbid) media. This technique, Monte Carlo radiation transfer (MCRT), is what makes up the bulk of this thesis and is described in depth

in the following sections.



**Figure 1.4:** Computer generated imagery using ray tracing. The Monte Carlo method is used to “compute radiance along ray paths between lights and the camera”, to generate CGI images [16].

## 1.2 Thesis Outline and Objective

This thesis concerns the development of advanced 3D light transport algorithm for various biophotonic and medical applications. The technique that is adopted to calculate the light transport for the majority of the thesis is the MCRT method. This method allows the tracking of photon packets through simulated 3D mediums, with the inclusion of multiple anisotropic scattering events along with the modelling of various other micro-physics that light may undergo in a medium.

This chapter details the background to the Monte Carlo method and its various application to a myriad of different fields.

## 1.3 Synopsis and Thesis Objectives

Again repeat first para -> talk about dev of MCRT and why use it i.e non invasive digital twin thing ilas mentioned. mcrt is flexible etc

Chapter two details the Monte Carlo radiation transport method that is used for the bulk of this thesis. Presented in this chapter are details of the algorithm and various code details that underpin the whole thesis. Details of speed up techniques such as parallelisation are also presented. Finally the code is validated against other results.

Chapter three demonstrates details the tissue ablation model. Discussion of the individual components of the model, alongside validation of the model against theoretical and experimental evidence is also presented.

Chapter four presents an adaptation to the regular Monte Carlo model so that it can model wave like properties of photons including diffraction and interference. The new algorithm is

validated against several theoretical expressions and experimental data. Finally the algorithm is used to compare Bessel beams and Gaussian beam in highly turbid media, to determine which beam performs better.

Chapter five details the modelling of a novel biomarker for cardiovascular disease, autofluorescence. The theoretical groundwork for the biomarker is outlined, along with discussion of how Monte Carlo radiation transport can model fluorescence. Presented alongside this is *ameombaM-CRT*, a Monte Carlo radiation transfer simplex algorithm used to determine concentrations of fluorophores in different layers of tissue for a given spectrum. Chapter six details ....

Finally chapter seven concludes this thesis and presents possible future avenues of research that could be undertaken.





# Bibliography

- [1] Abdulmotaleb El Saddik. Digital twins: The convergence of multimedia technologies. *IEEE MultiMedia*, 25(2):87–92, 2018.
- [2] Edmond D Cashwell and Cornelius Joseph Everett. A practical manual on the monte carlo method for random walk problems. 1959.
- [3] DWO Rogers and AF Bielajew. Monte carlo techniques of electron and photon transport for radiation dosimetry. *The dosimetry of ionizing radiation*, 3:427–539, 1990.
- [4] Lee Badger. Lazzarini’s lucky approximation of  $\pi$ . *Mathematics Magazine*, 67(2):83–91, 1994.
- [5] Petr Beckmann. *A history of Pi*. St. Martin’s Griffin, 2015.
- [6] Georges-Louis Leclerc Buffon. *Histoire naturelle générale et particulière*, volume 18. de l’Imprimerie de F. Dufart, 1785.
- [7] Peter Jäckel. *Monte Carlo methods in finance*. J. Wiley, 2002.
- [8] David B Hertz. Risk analysis in capital investment. *Harvard Business Review*, 42(1):95–106, 1964.
- [9] Jasper Vivian Wall and Charles R Jenkins. *Practical statistics for astronomers*. Cambridge University Press, 2012.
- [10] James T. Kajiya. The rendering equation. *SIGGRAPH Comput. Graph.*, 20(4):143–150, August 1986.
- [11] Robert L. Cook, Thomas Porter, and Loren Carpenter. Distributed ray tracing. *SIGGRAPH Comput. Graph.*, 18(3):137–145, January 1984.
- [12] Thomas P Robitaille. Hyperion: an open-source parallelized three-dimensional dust continuum radiative transfer code. *Astronomy & Astrophysics*, 536:A79, 2011.
- [13] Tim Harries. Torus: Radiation transport and hydrodynamics code. *Astrophysics Source Code Library*, 2014.
- [14] Ronan M Valentine, Christian TA Brown, Kenneth Wood, Harry Moseley, and Sally Ibbotson. Monte carlo modeling of in vivo protoporphyrin ix fluorescence and singlet oxygen production during photodynamic therapy for patients presenting with superficial basal cell carcinomas. *Journal of Biomedical Optics*, 16(4):048002, 2011.

- [15] C.L Campbell, K. Wood, R.M. Valentine, C.T.A Brown, and H. Moseley. Monte carlo modelling of daylight activated photodynamic therapy. *Physics in Medicine & Biology*, 60(10):4059, 2015.
- [16] Matt Pharr, Wenzel Jakob, and Greg Humphreys. *Physically based rendering: From theory to implementation*. Morgan Kaufmann, 2016.