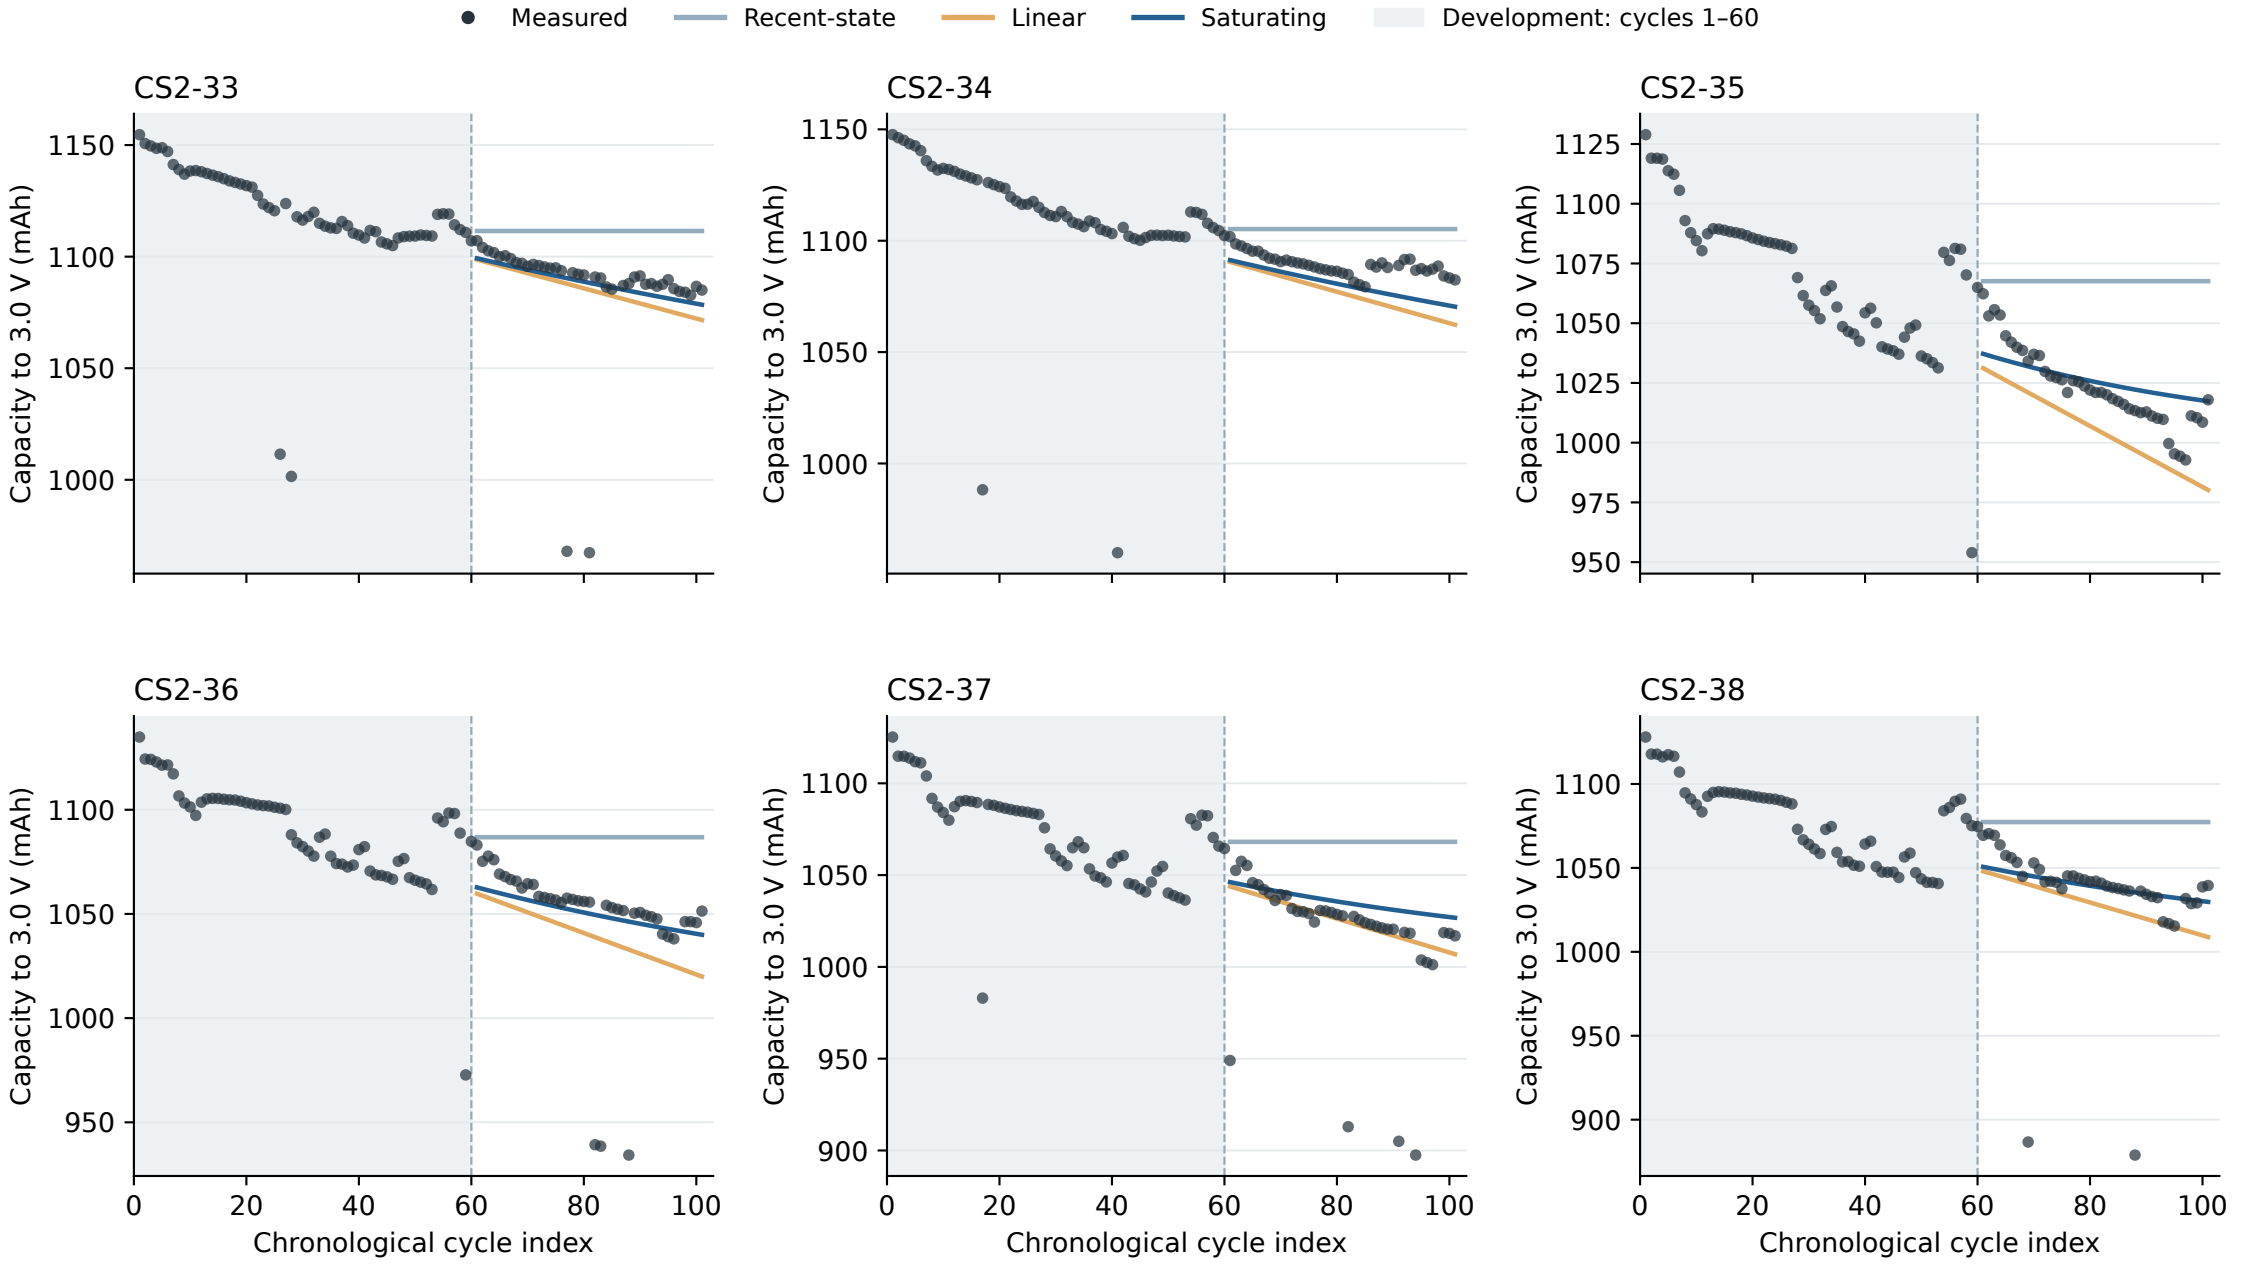

Additional-cell capacity diagnostics use the same 3.0-V analysis endpoint and the fixed chronological horizon.