


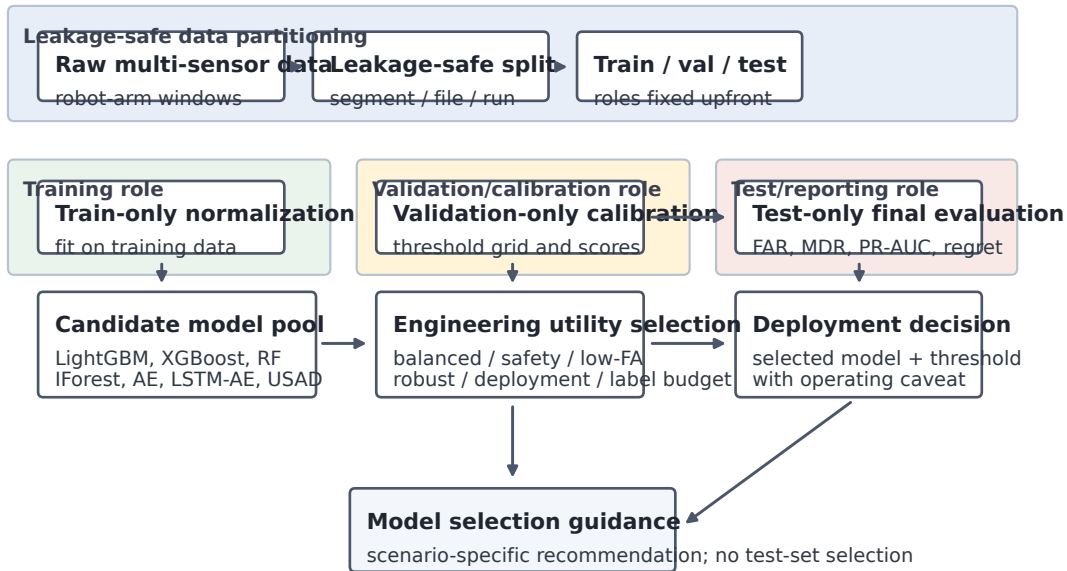

Decision workflow: model and threshold are selected only on validation/calibration data; held-out test data are used once for final reporting.