


ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 10x1 C-FINE Cuff - 16 Contact	12/16/2014	
-	2	Anode Strip Addition	9/13/2015	

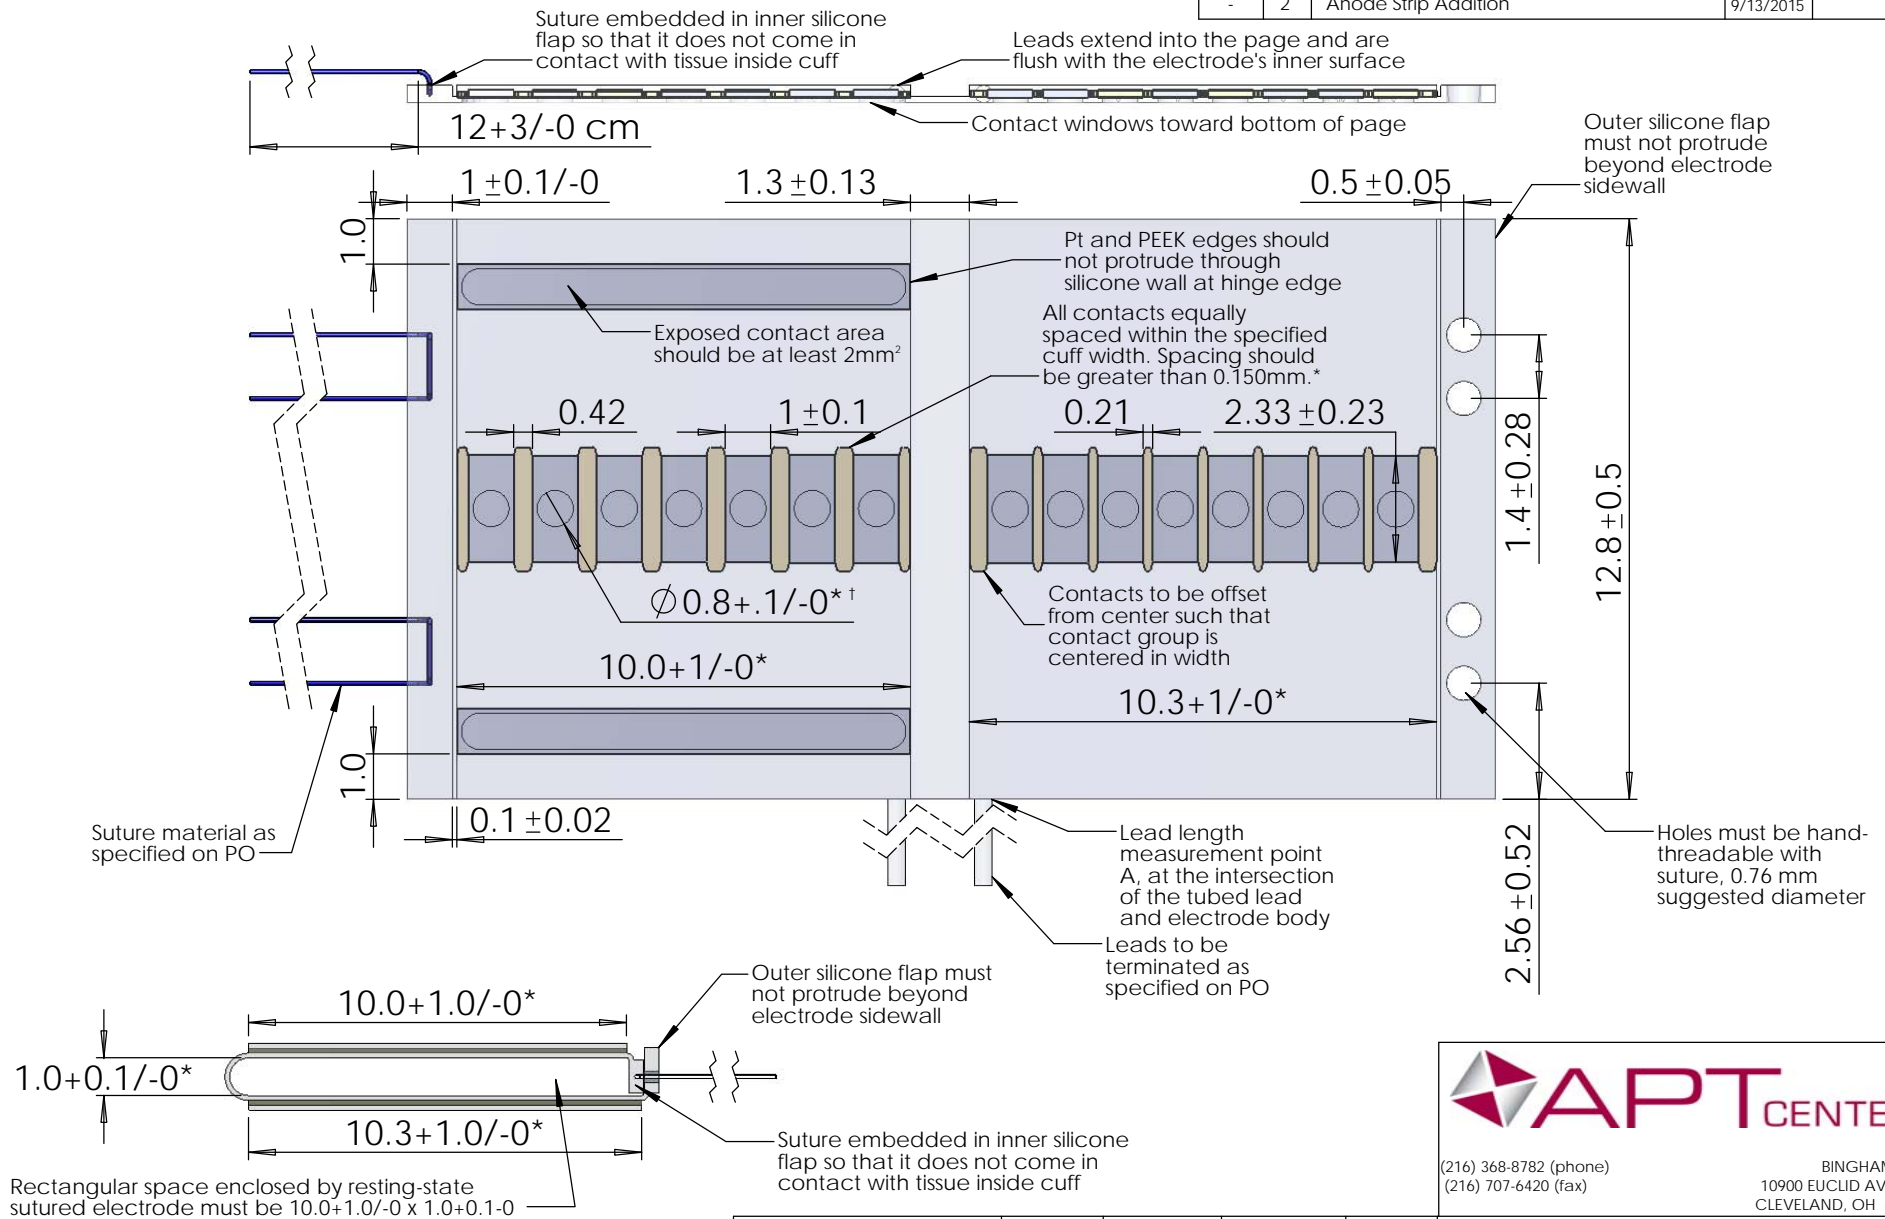

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	D. Tyler		
MFG APPR.			
Q.A.	E. Panek		
COMMENTS:			



(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

10mm x 1mm C-FINE Cuff - 16 Contact


P/N: 004-33-022

SIZE **A** DWG. NO. 004-22-022

REV. 2

SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 10x1.5 C-FINE Cuff - 16 Contact	12/16/2014	
-	2	Anode Strip Addition	9/13/2015	

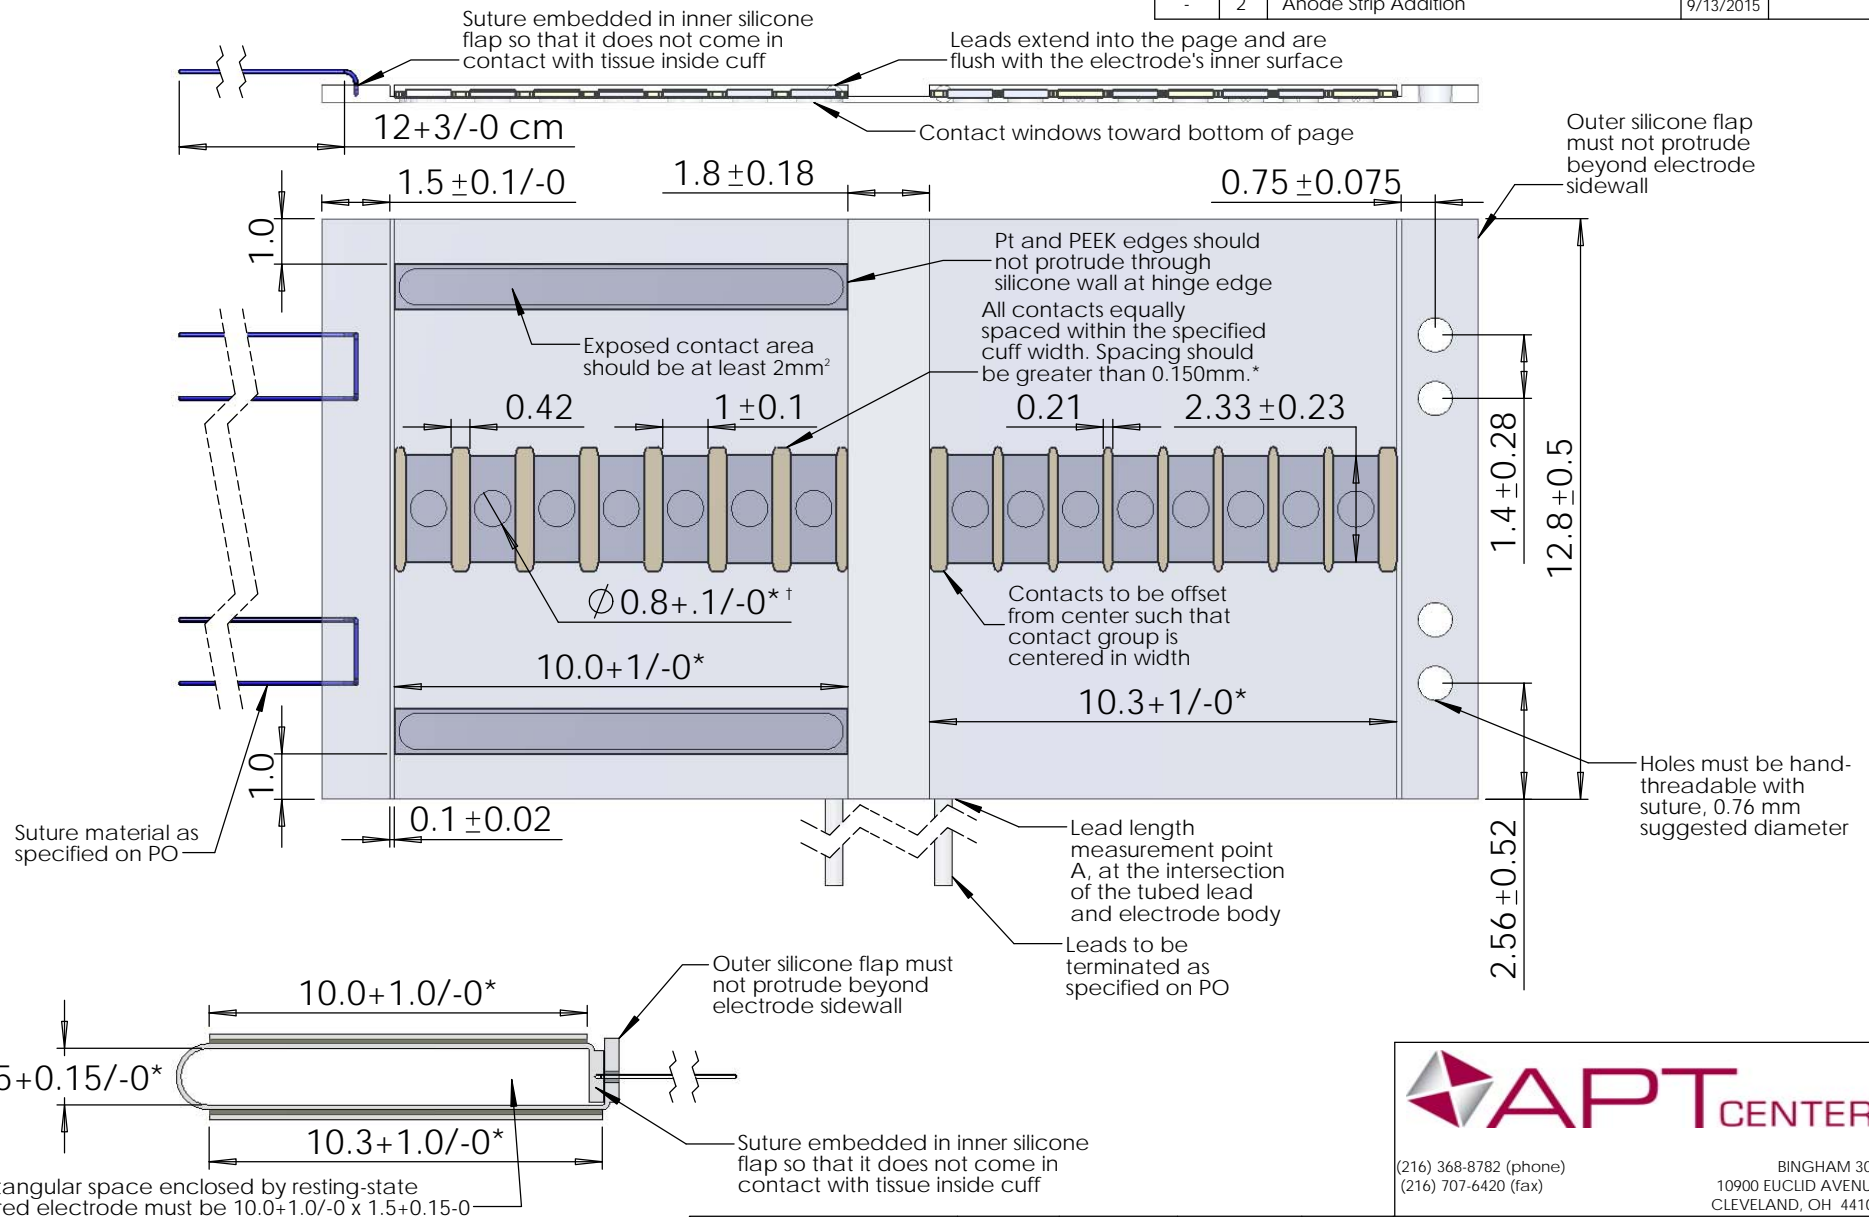

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL

THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED

TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*)

DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	D. Tyler		
MFG APPR.			
Q.A.	E. Panek		
COMMENTS:			


10mm x 1.5mm C-FINE Cuff - 16 Contact

P/N: 004-33-023

SIZE A DWG. NO. 004-22-023

REV. 2

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 15x1.5 C-FINE Cuff - 16 Contact	12/16/2014	
-	2	Anode Strip Addition	9/13/2015	

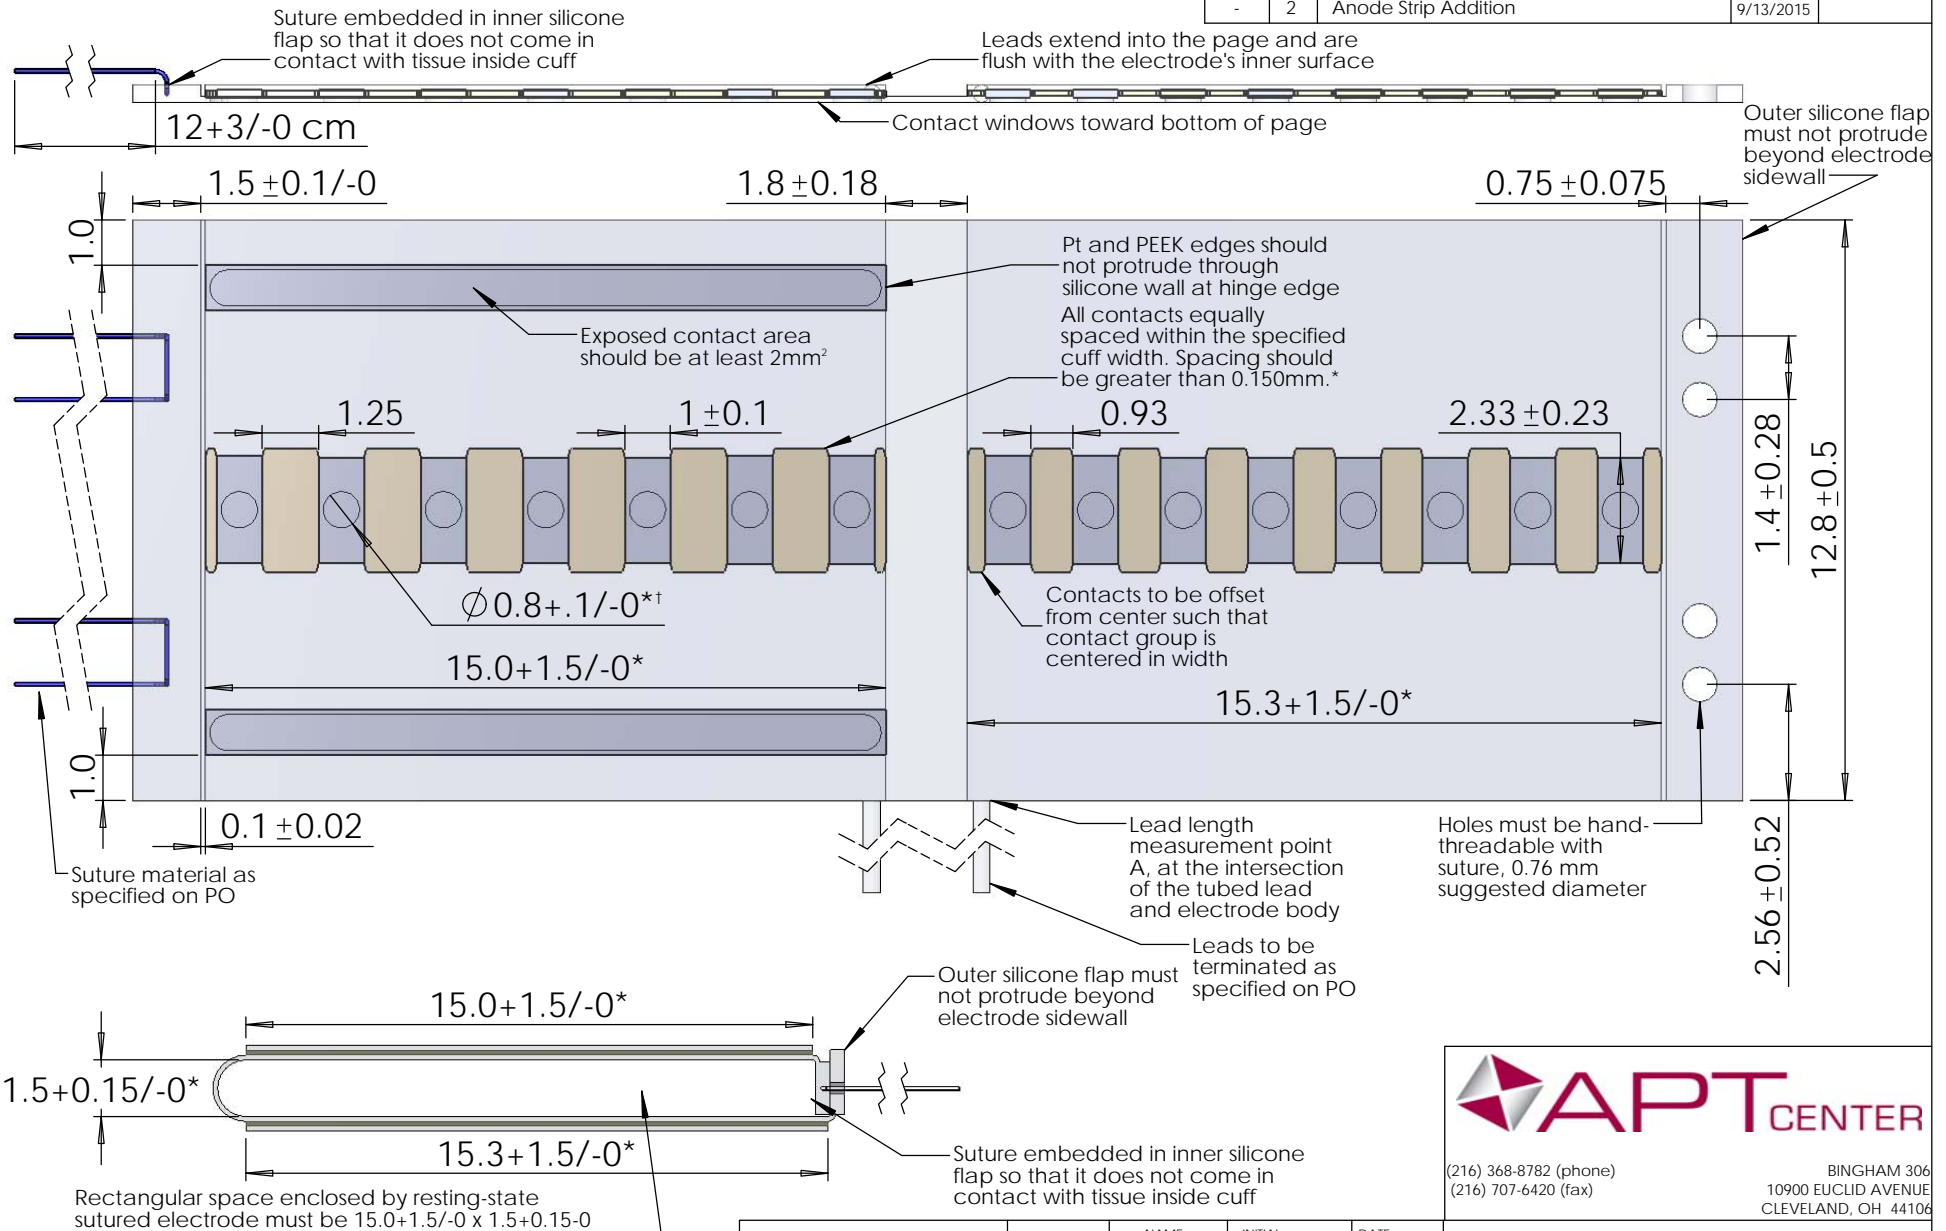

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.




DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	D. Tyler		
MFG APPR.			
Q.A.	E. Panek		
COMMENTS:			

APT CENTER
(216) 368-8782 (phone)
(216) 707-6420 (fax)
BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

15mm x 1.5mm C-FINE Cuff - 16 Contact			
P/N: 004-33-024			
SIZE A	DWG. NO. 004-22-024	REV. 2	SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 5x1 C-FINE Cuff - 8 Contact	12/16/2014	

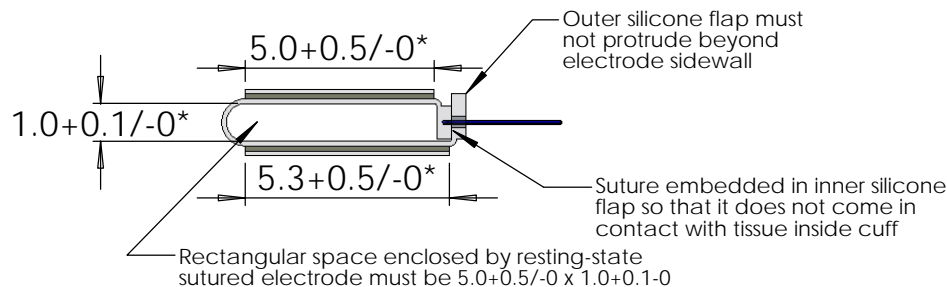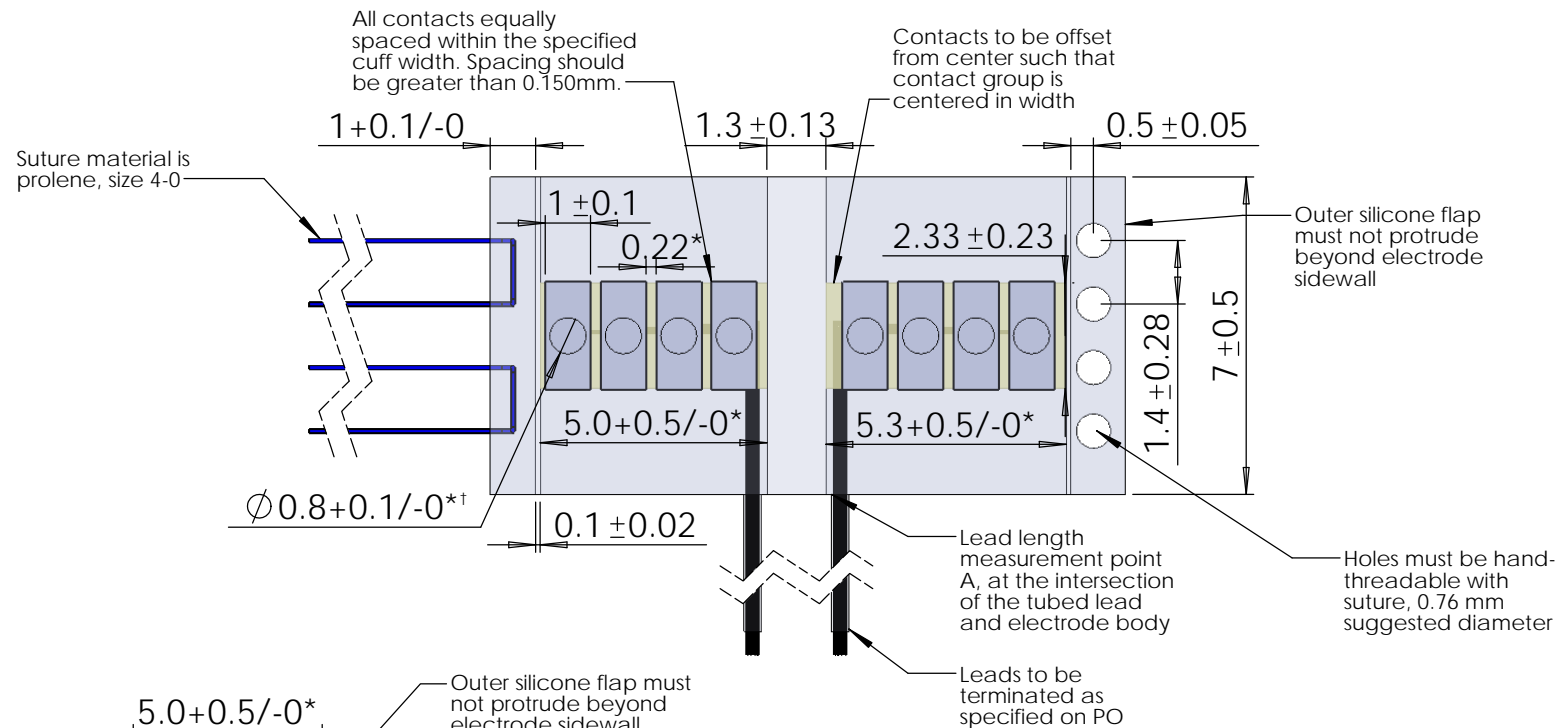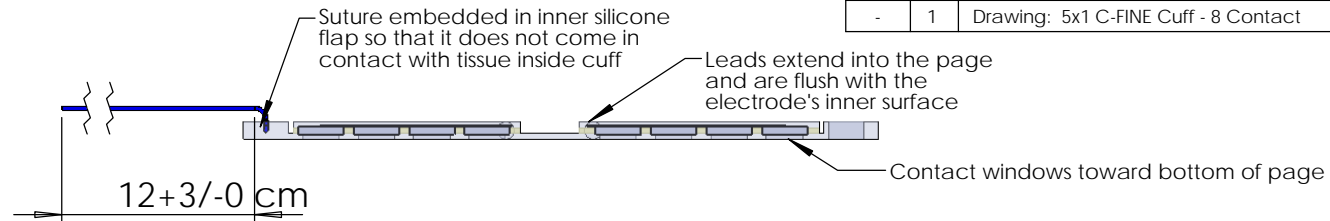

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are 4-0 prolene material and are embedded in silicone flap as marked.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED



TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")

DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

5mm x 1mm C-FINE Cuff - 8 Contact			
P/N: 004-33-008			
SIZE A	DWG. NO. 004-22-008	REV. 1	
			SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 6x1 C-FINE Cuff - 10 Contact	12/16/2014	

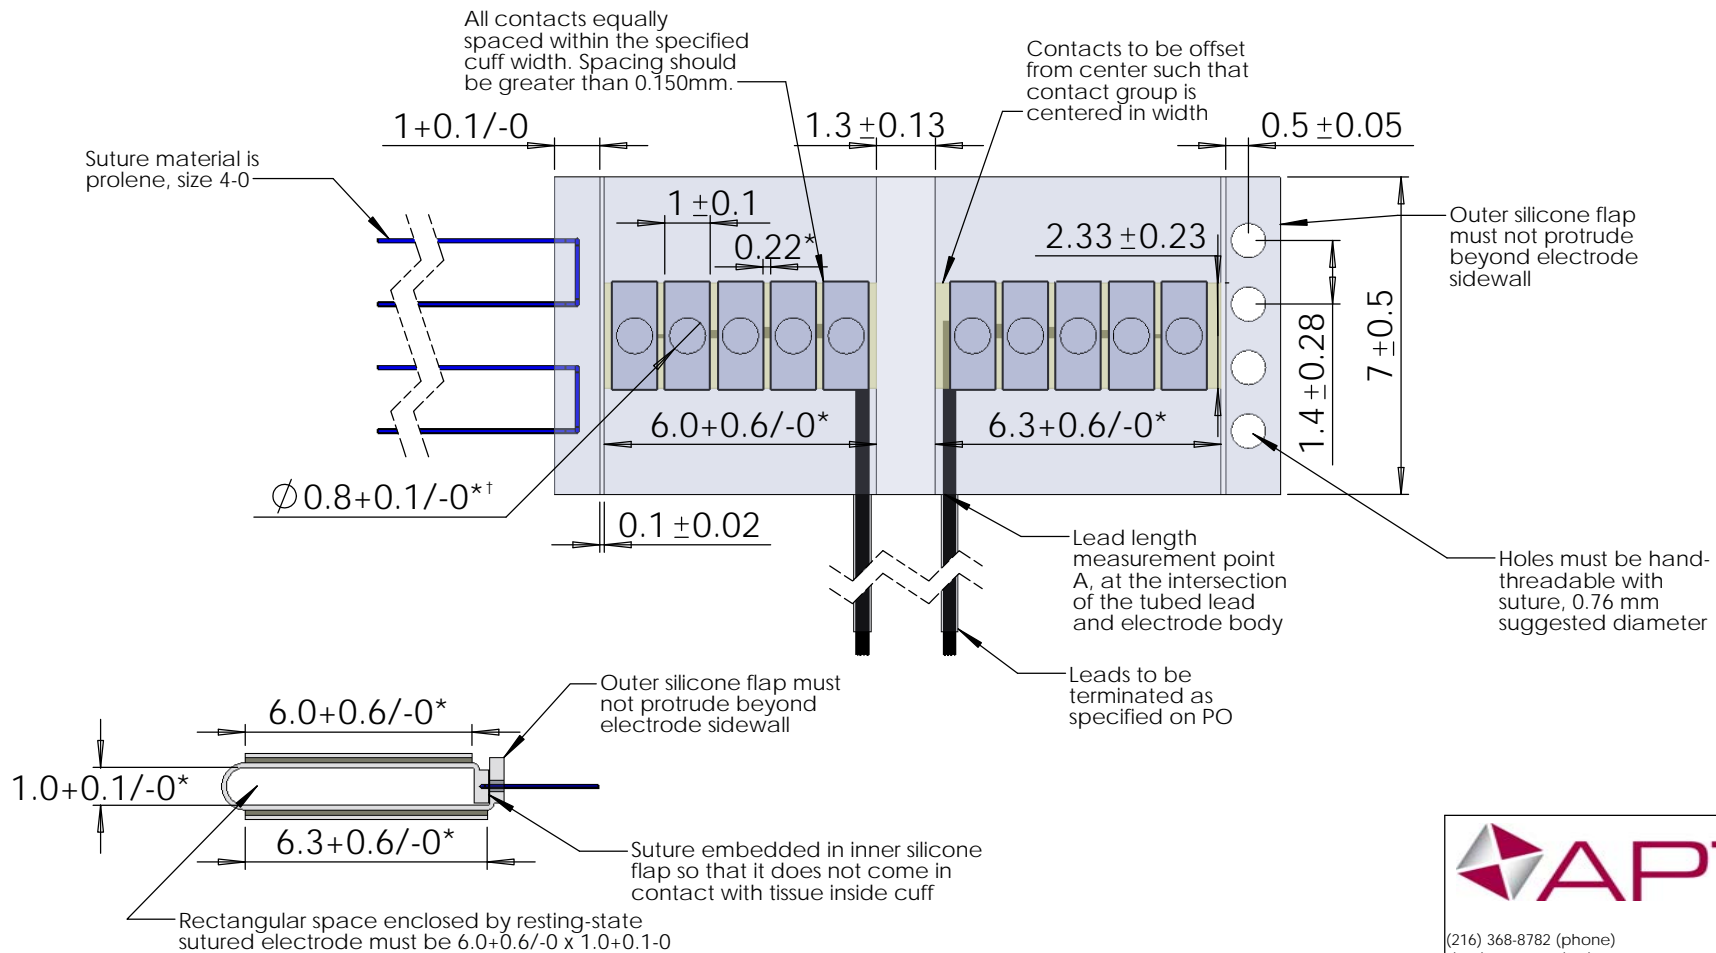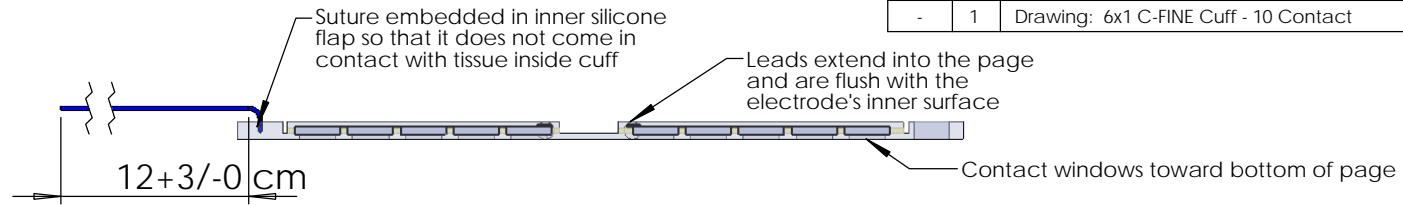

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are 4-0 prolene material and are embedded in silicone flap as marked.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED

TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")


DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

6mm x 1mm C-FINE Cuff - 10 Contact
P/N: 004-33-009

SIZE	DWG. NO.	REV.
A	004-22-009	1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 7x1 C-FINE Cuff - 12 Contact	12/16/2014	

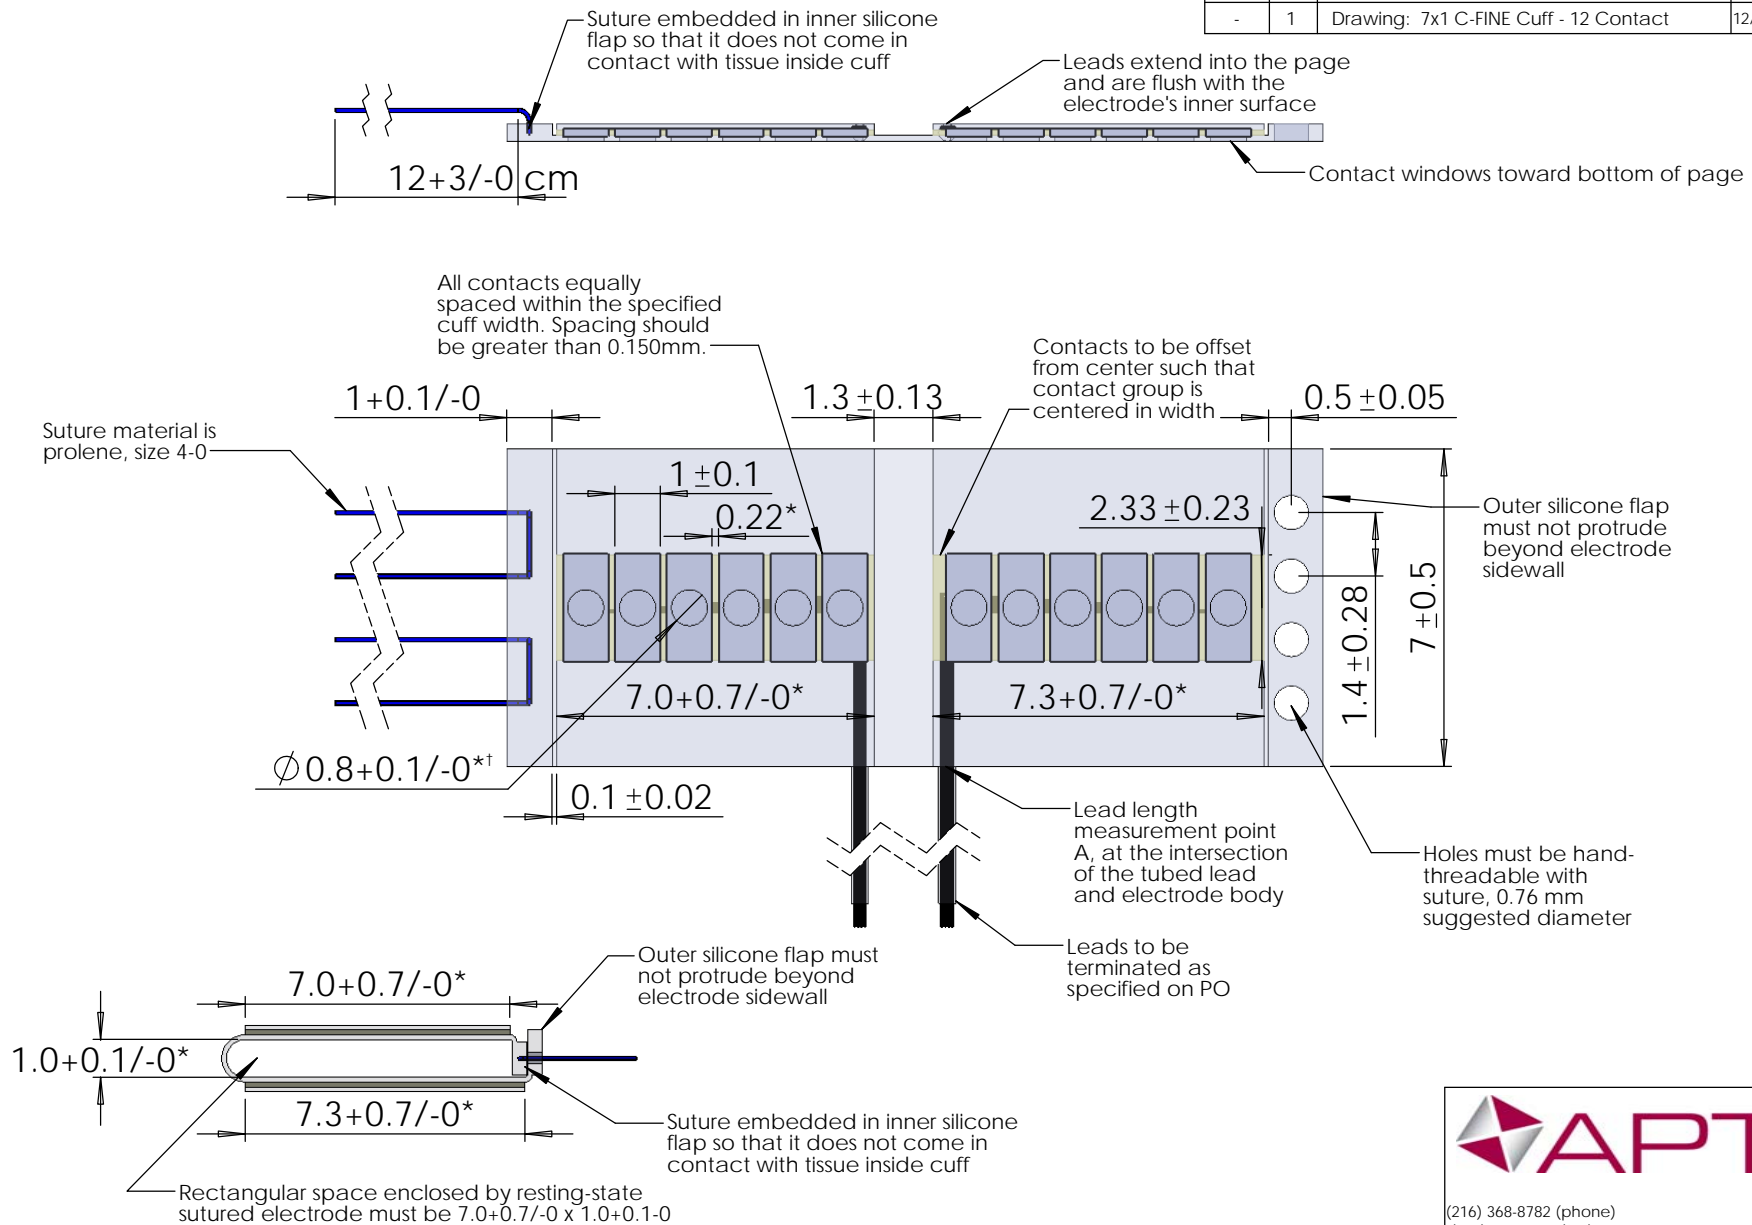

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are 4-0 prolene material and are embedded in silicone flap as marked.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.




DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

APT CENTER
(216) 368-8782 (phone)
(216) 707-6420 (fax)
BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

7mm x 1mm C-FINE Cuff - 12 Contact
P/N: 004-33-010
SIZE **A** DWG. NO. 004-22-010 REV. 1
SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	3	Drawing: 10x1 C-FINECuff - 8 Contact	12/16/2014	

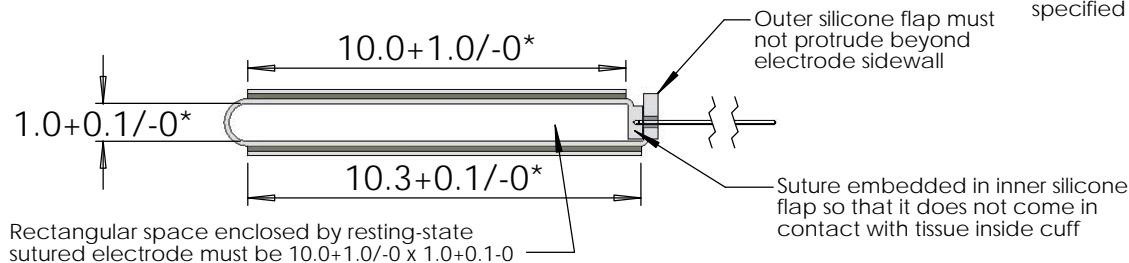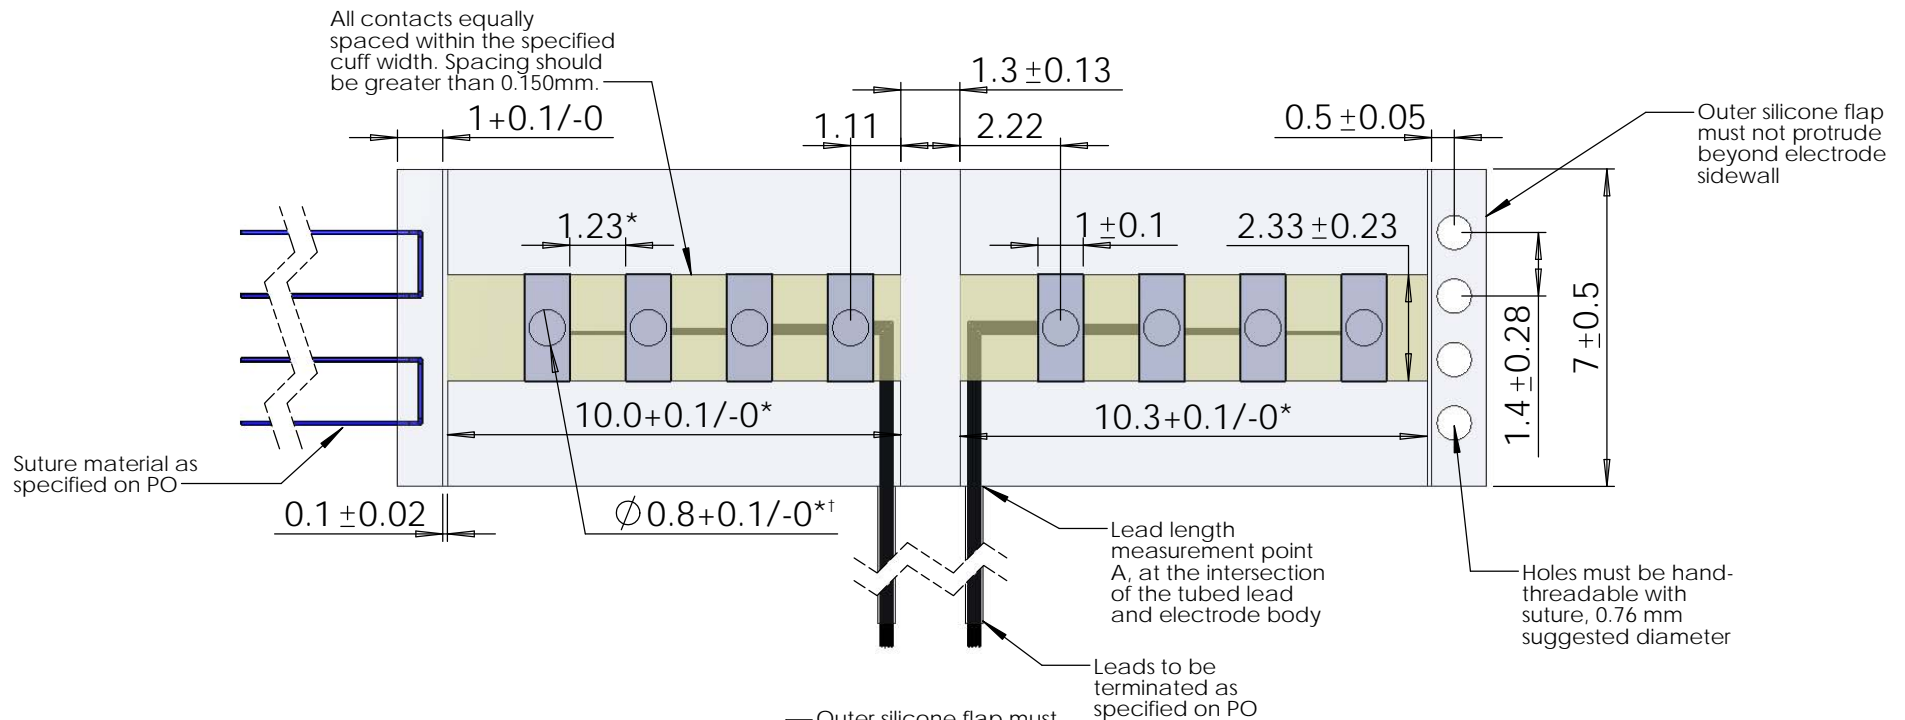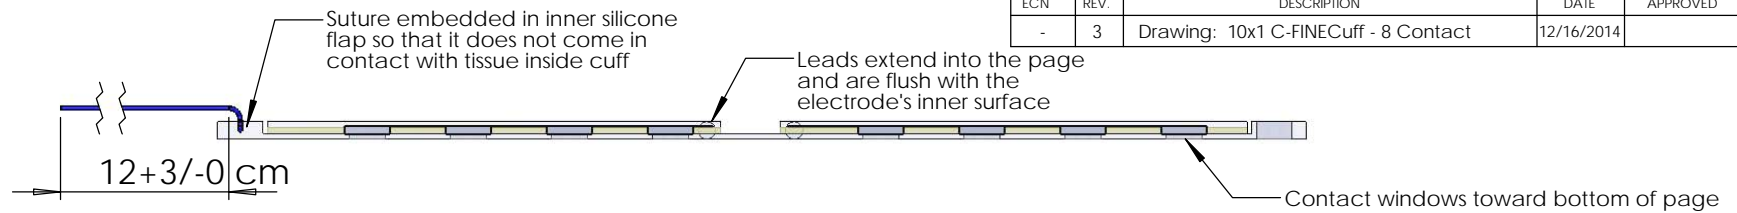

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			




10mm x 1mm C-FINE Cuff - 8 Contact

P/N: 004-33-001

SIZE **A** DWG. NO. 004-22-001

REV. 3

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 10x1 C-FINE Cuff - 16 Contact	12/16/2014	

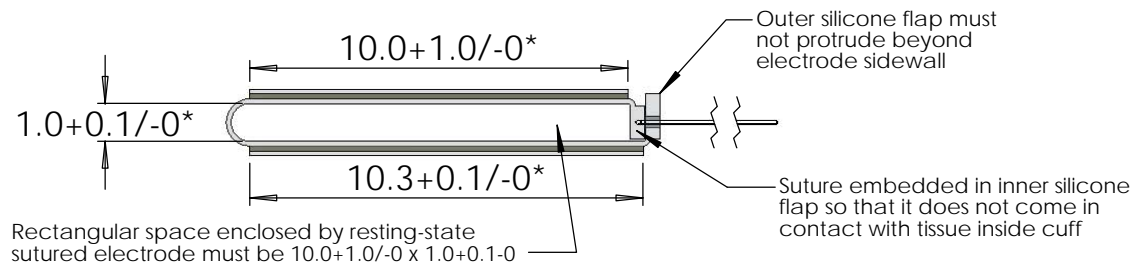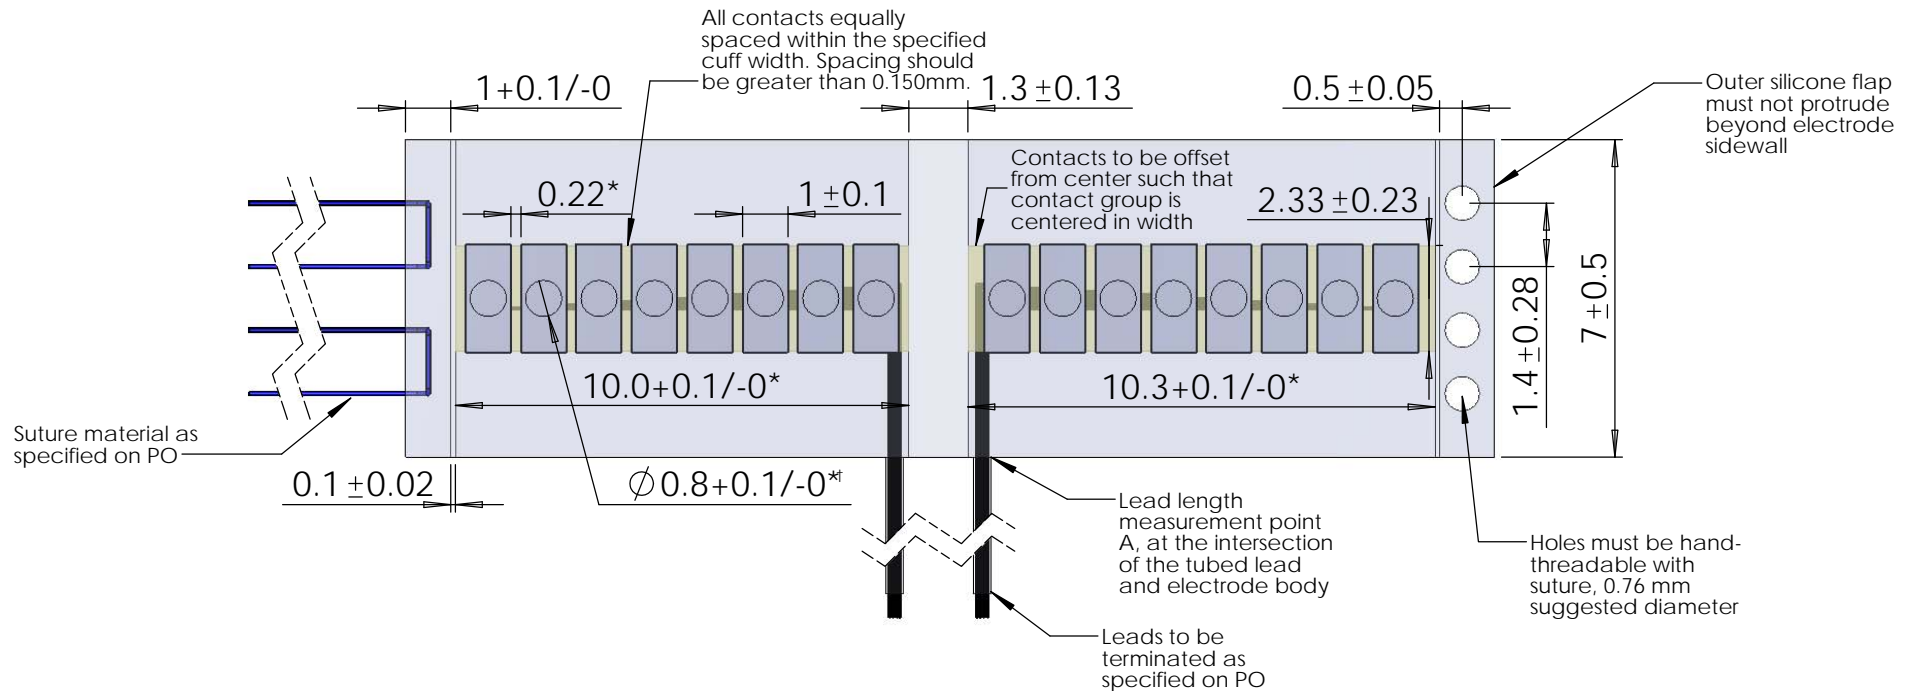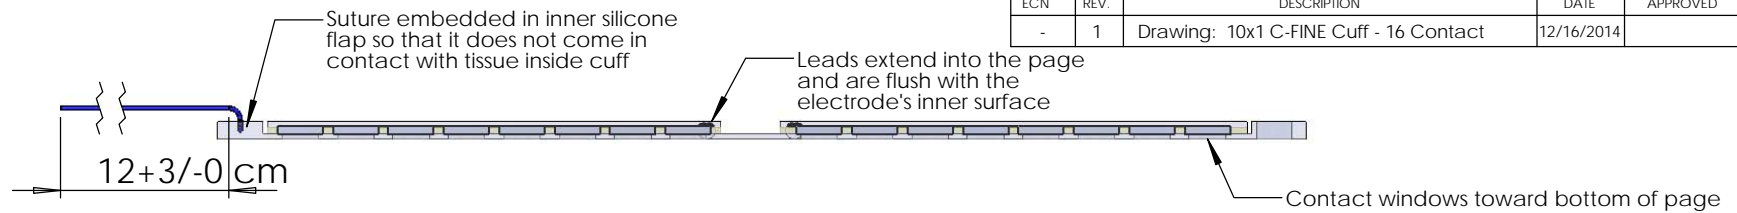

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

10mm x 1mm C-FINE Cuff - 16 Contact




P/N: 004-33-005

SIZE **A** DWG. NO. 004-22-005

REV. 1

SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	3	Drawing: 10x1.5 C-FINE Cuff - 8 Contact	12/16/2014	

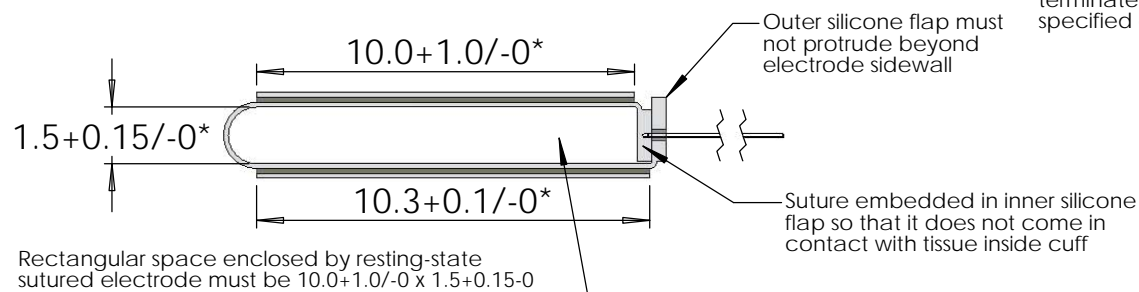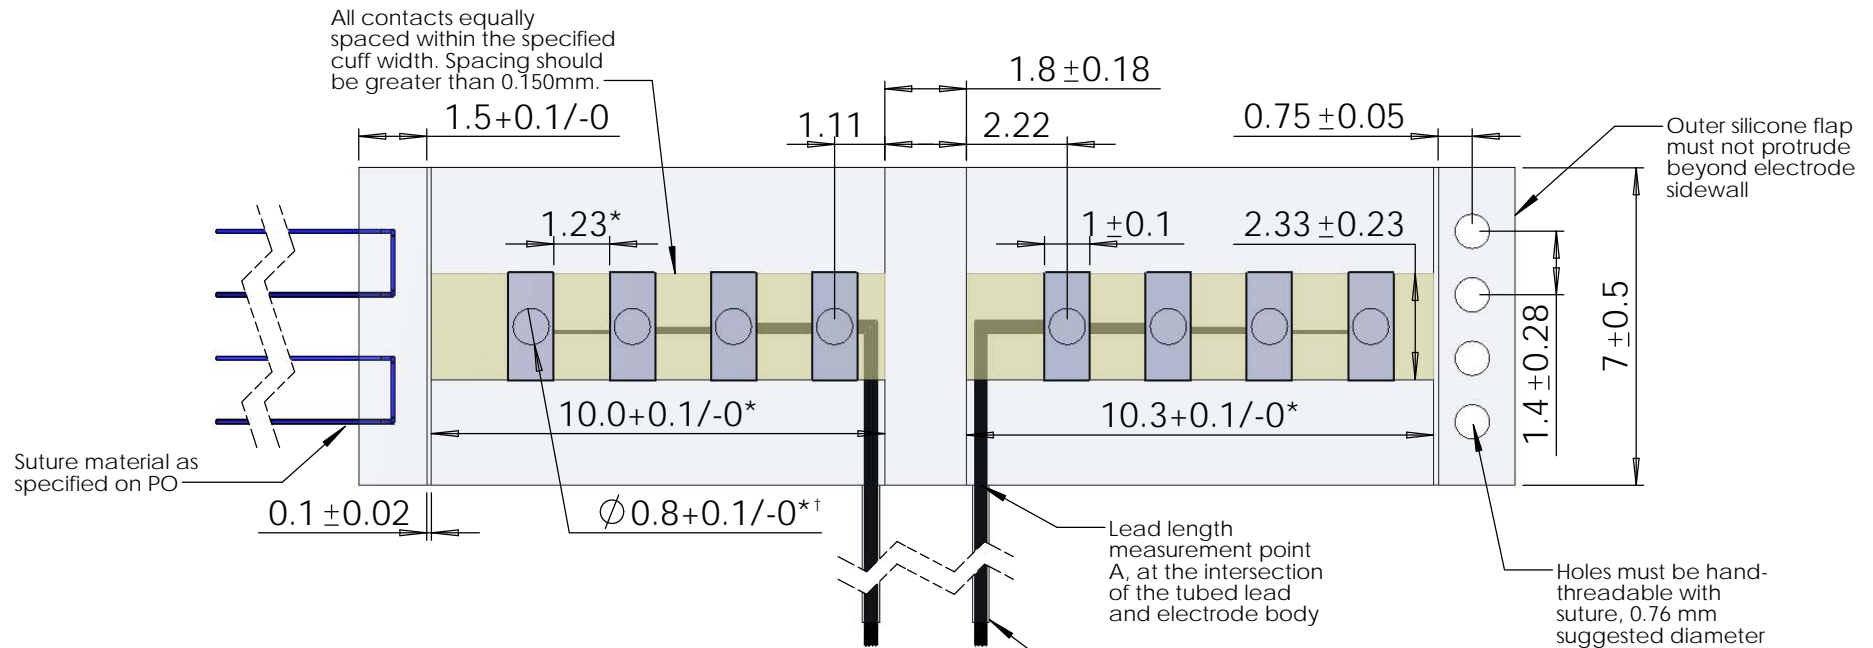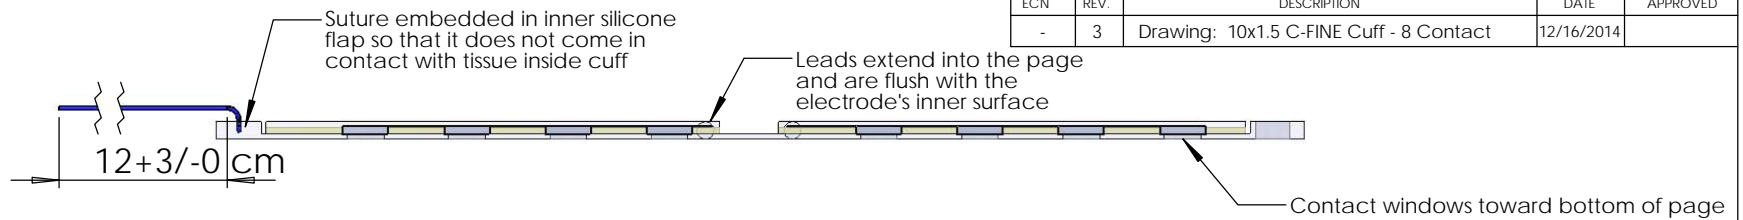

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED

TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")

DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.




	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

10mm x 1.5mm C-FINE Cuff - 8 Contact

P/N: 004-33-002

SIZE	DWG. NO.	REV.
A	004-22-002	3

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 10x1.5 C-FINE Cuff - 16 Contact	12/16/2014	

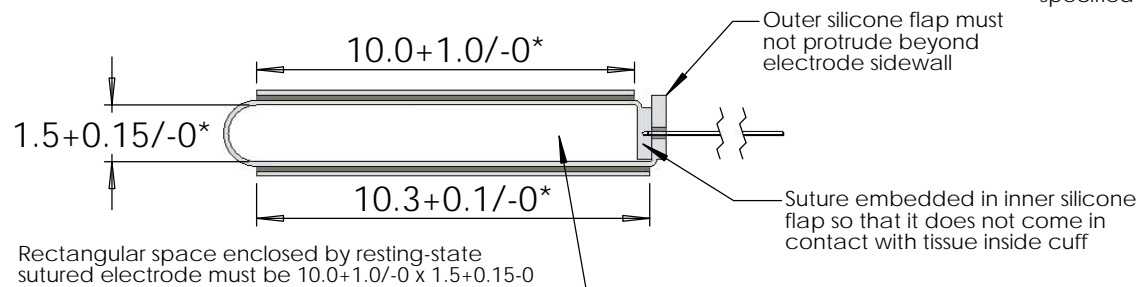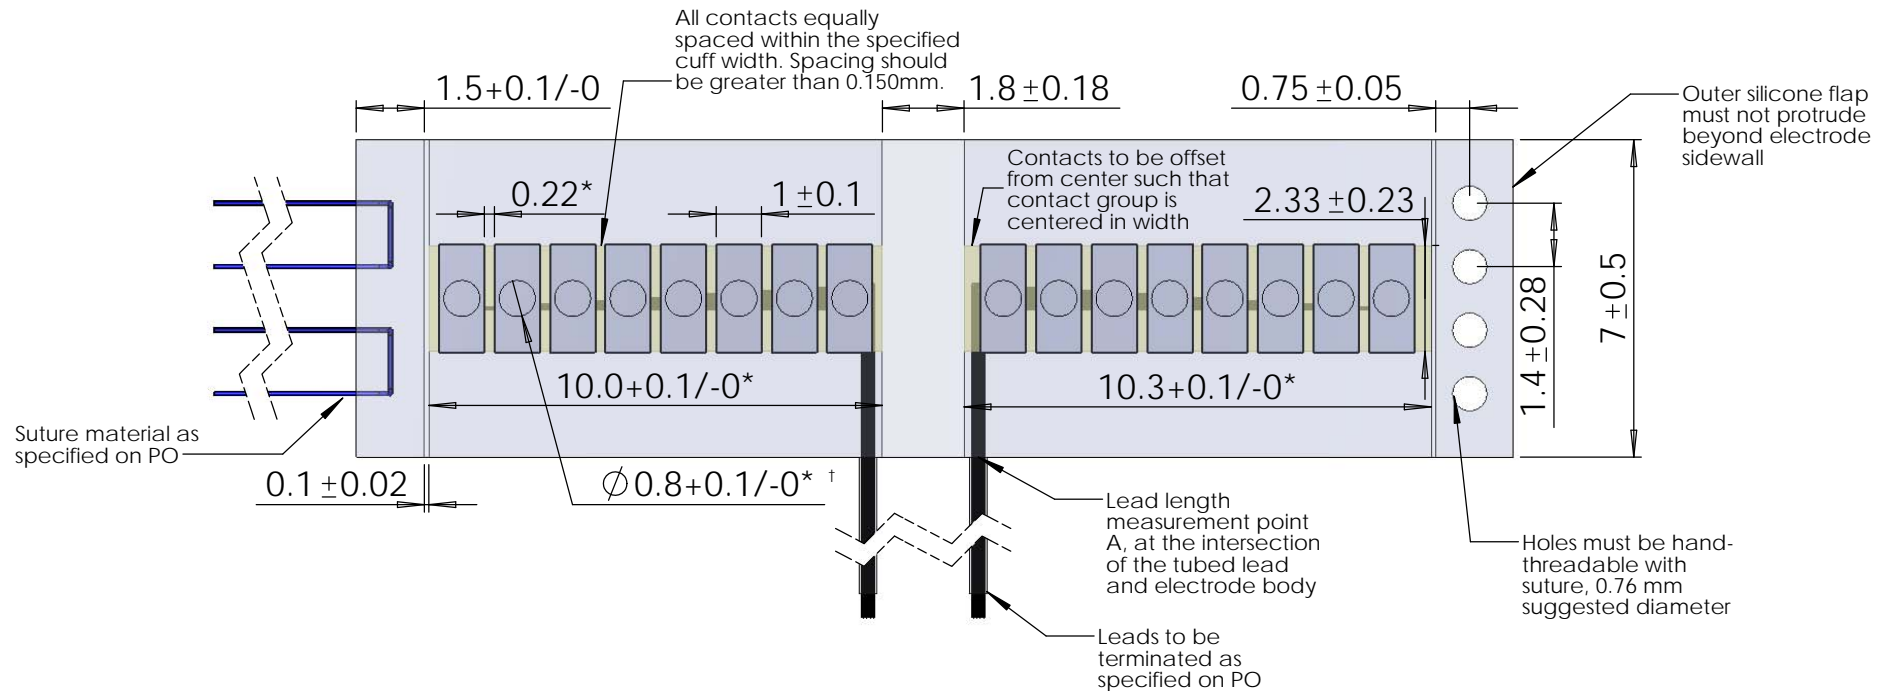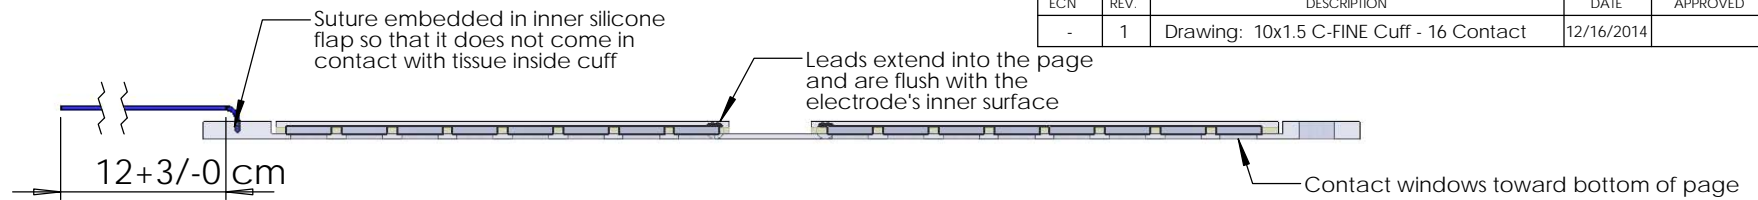

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED

TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)

DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			



(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106


10mm x 1.5mm C-FINE Cuff - 16 Contact

P/N: 004-33-006

SIZE A DWG. NO. 004-22-006

REV. 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	3	Drawing: 15x1.5 C-FINE Cuff - 8 Contact	12/16/2014	

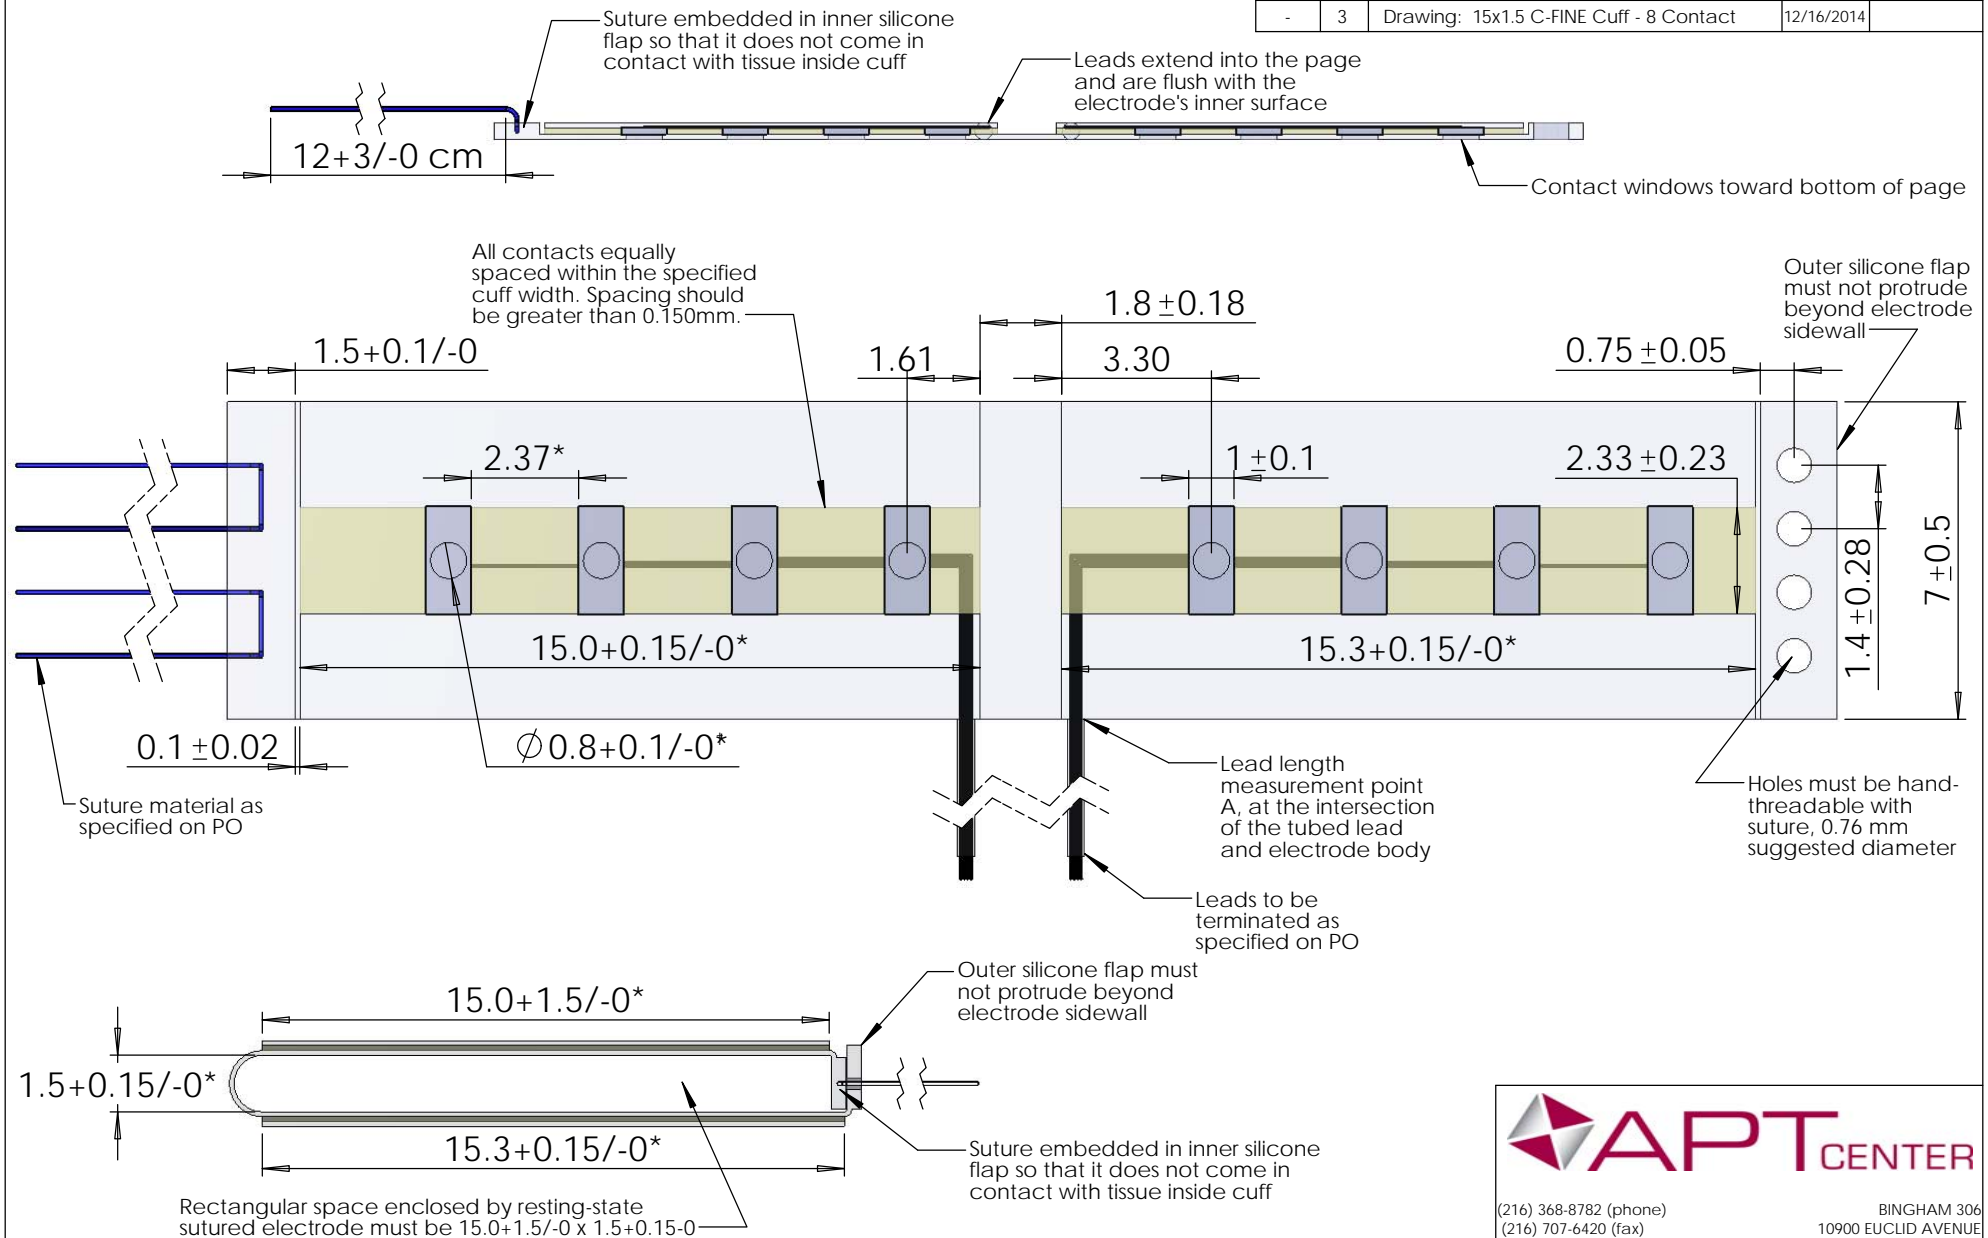

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK ("*")
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

15mm x 1.5mm C-FINE - 8 Contact


P/N: 004-33-003

SIZE **A** DWG. NO. 004-22-003

REV. 3

SHEET 1 OF 1

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 15x1.5 C-FINE Cuff - 16 Contact	12/16/2014	

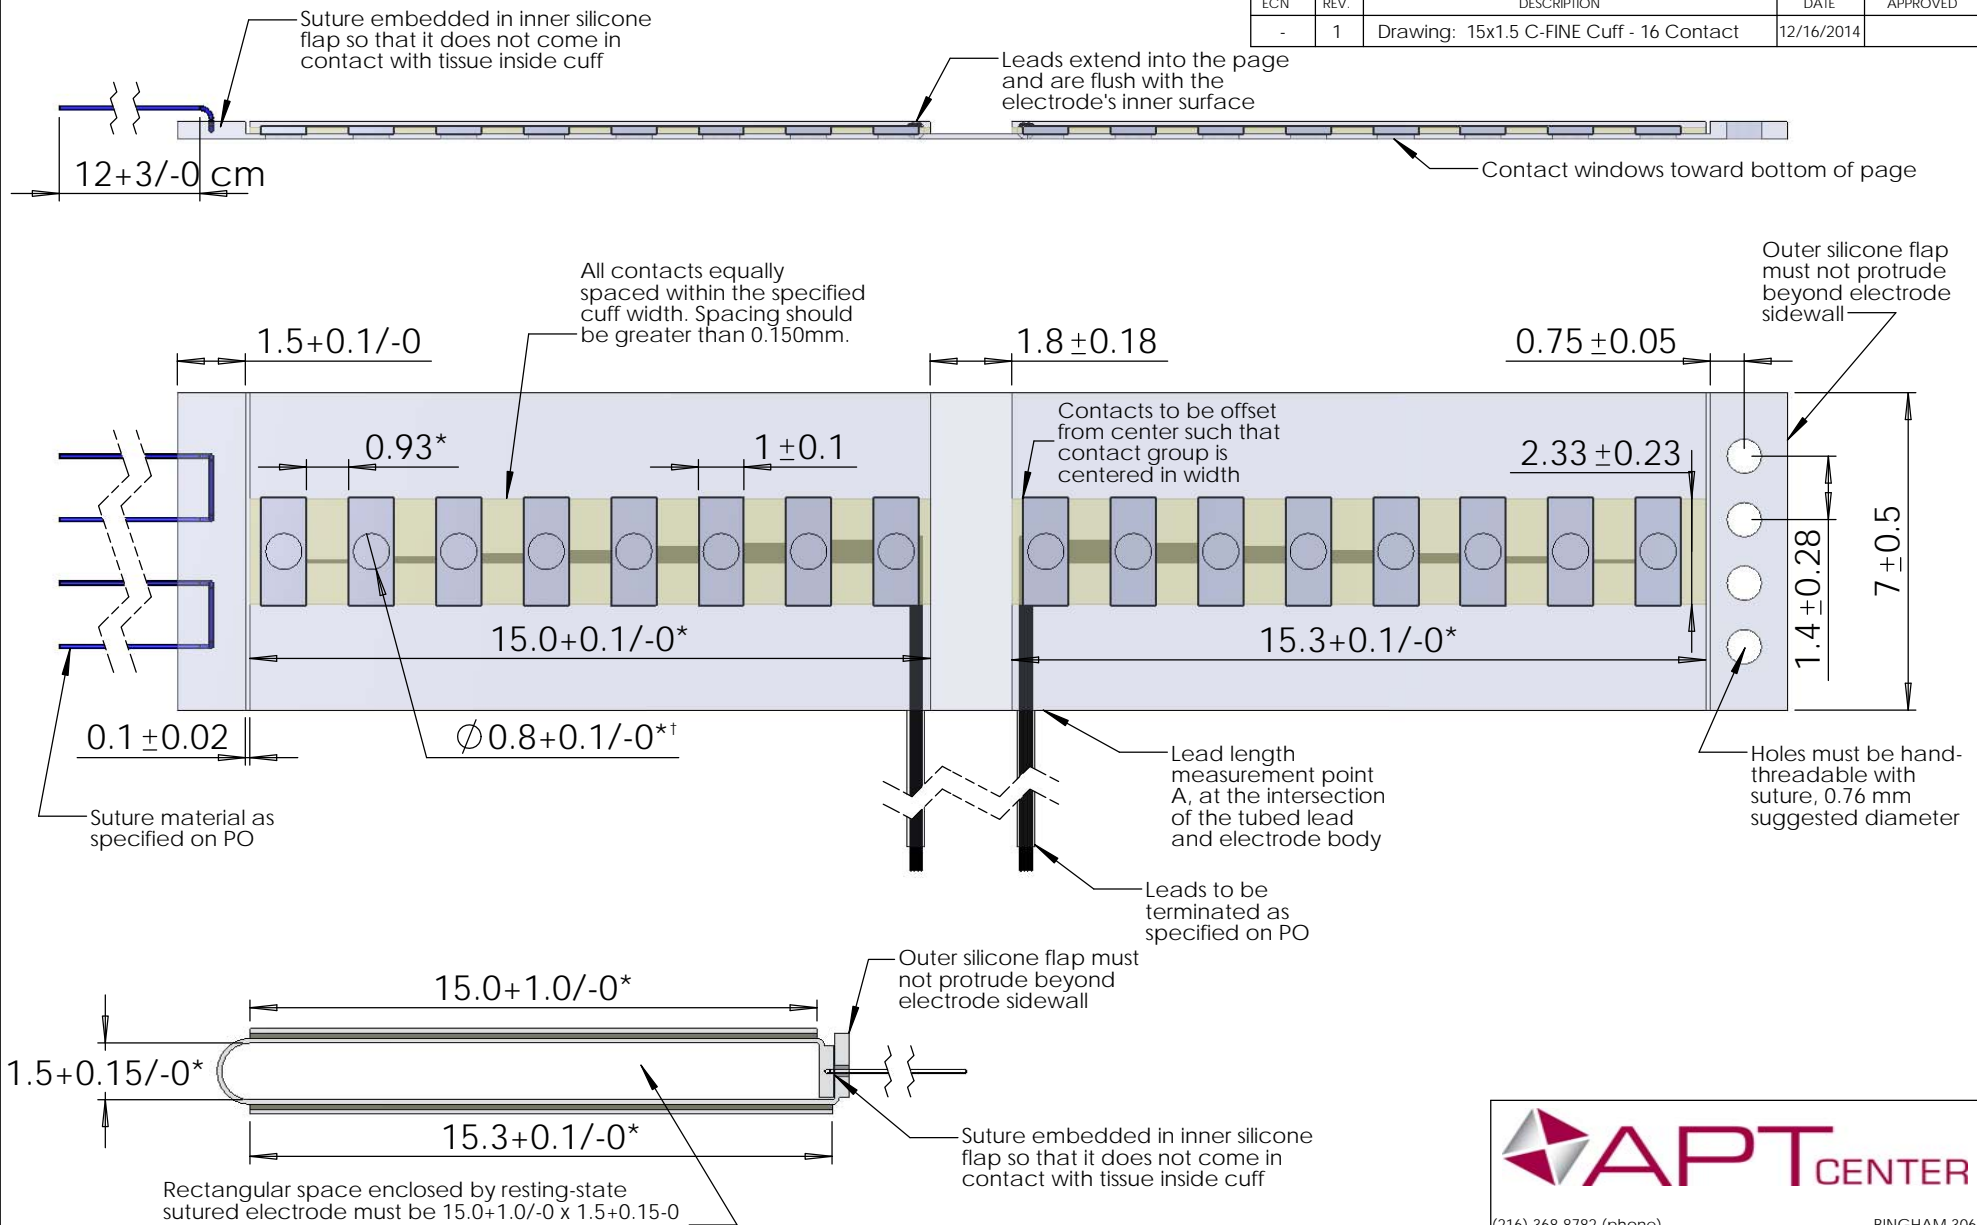

NOTES:
Critical dimensions are marked with an asterisk symbol: "*". Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL.

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	D. Tyler		
COMMENTS:			

(216) 368-8782 (phone)
(216) 707-6420 (fax)

BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

15mmx 1.5mm C-FINE Cuff - 16 Contact

P/N: 004-33-007

SIZE	DWG. NO.	REV.
A	004-22-007	1

SHEET 1 OF 1

[illegible]

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS
DRAWING IS THE SOLE PROPERTY OF
APT CENTER. ANY
REPRODUCTION IN PART OR AS A WHOLE
WITHOUT THE WRITTEN PERMISSION OF
APT CENTER IS PROHIBITED.


DIMENSIONS ARE IN
MILLIMETERS
UNLESS OTHERWISE SPECIFIED

TOLERANCES ON ALL CRITICAL
DIMENSIONS ARE MARKED WITH
AN ASTERISK (**)

DIMENSIONS WITHOUT AN
ASTERISK ARE NON-CRITICAL.

15mm x 2mm C-FINE Cuff - 16 Contact			
P/N: 004-33-011			
SIZE A	DWG: NO 004-22-011		REV 1
		SHEET 1 OF 1	



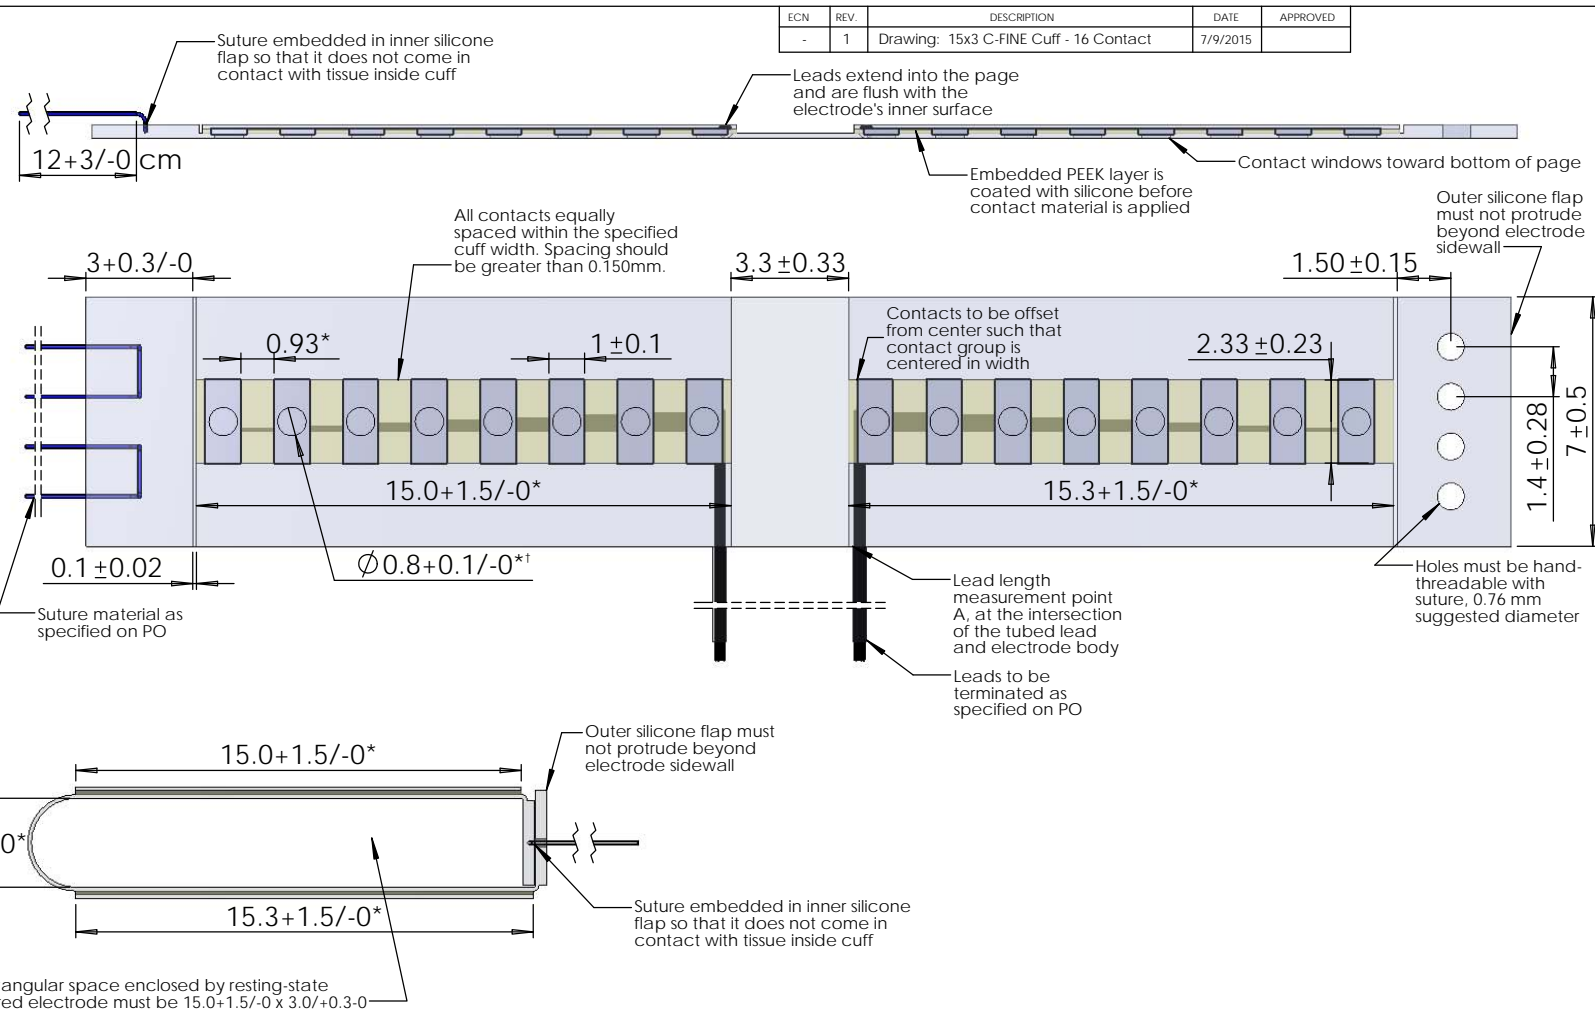

NOTES:
Critical dimensions are marked with an asterisk symbol: *. Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	E. Panek		
COMMENTS:			

15mm x 3mm C-FINE Cuff - 16 Contact

P/N: 004-33-012


SIZE A DWG. NO. 004-22-012

REV. 1

SHEET 1 OF 1

APT CENTER
(216) 368-8782 (phone)
(216) 707-6420 (fax)
BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

ECN	REV.	DESCRIPTION	DATE	APPROVED
-	1	Drawing: 20x3 C-FINE Cuff - 16 Contact	7/9/2015	
-	2	Contact spacing updated	10/14/2015	

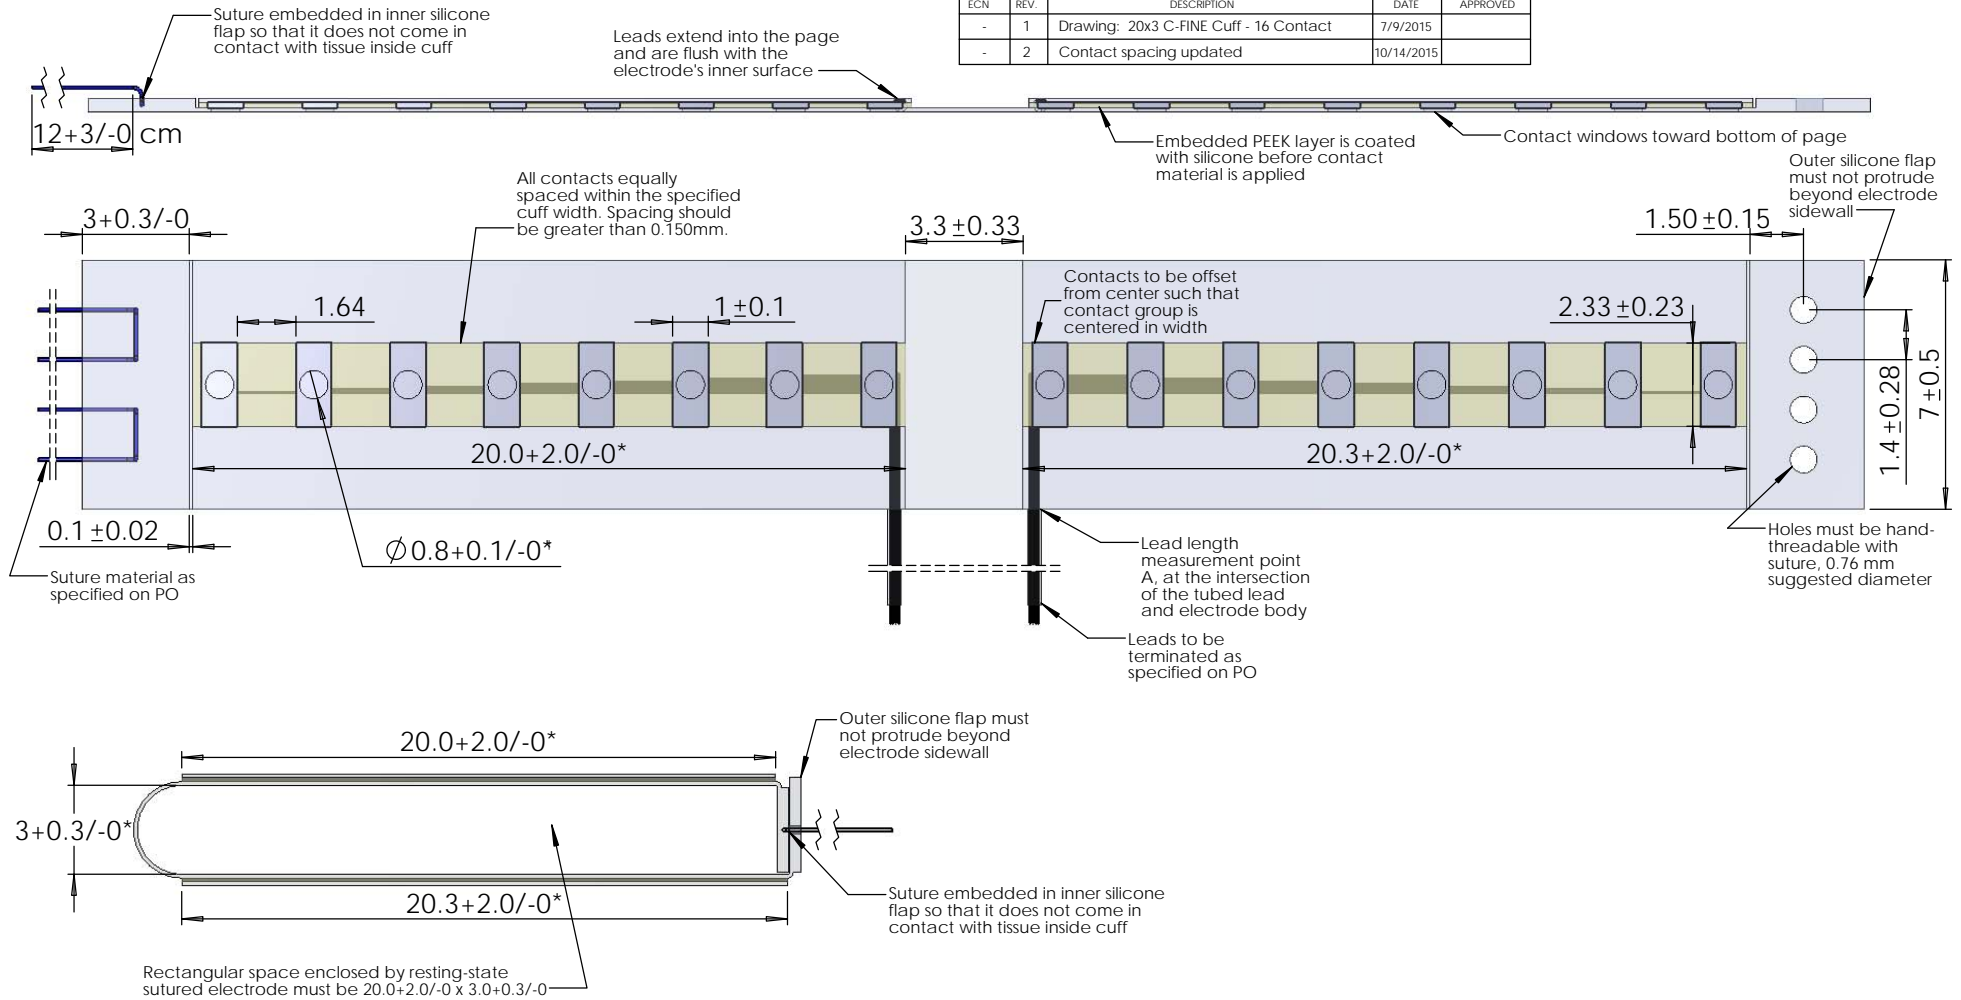

NOTES:
Critical dimensions are marked with an asterisk symbol: *. Critical dimensions must be inspected and certified to be within tolerance.
Sutures are embedded in silicone flap as marked. Size is surgeon selected and specified on the PO.
† Contact window cut-outs are to be centered horizontally on contact metal

PROPRIETARY AND CONFIDENTIAL
THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF APT CENTER. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF APT CENTER IS PROHIBITED.

DIMENSIONS ARE IN MILLIMETERS UNLESS OTHERWISE SPECIFIED
TOLERANCES ON ALL CRITICAL DIMENSIONS ARE MARKED WITH AN ASTERISK (*)
DIMENSIONS WITHOUT AN ASTERISK ARE NON-CRITICAL

	NAME	INITIAL	DATE
DRAWN	J. Dunning		
CHECKED			
ENG APPR.	B. Boggs		
MFG APPR.			
Q.A.	E. Panek		
COMMENTS:			

20mm x 3mm C-FINE Cuff - 16 Contact

P/N: 004-33-013

SIZE A DWG. NO. 004-22-013

SHEET 1 OF 1

APT CENTER
(216) 368-8782 (phone)
(216) 707-6420 (fax)
BINGHAM 306
10900 EUCLID AVENUE
CLEVELAND, OH 44106

