

Sleeve print proof — Route B, pure white board

BRANDING UPDATED 9 SEPTEMBER 2026 · GEOMETRY SUPERSEDED · NOT FOR PRINT

DO NOT SEND TO A PRINTER. THE GEOMETRY ON THESE PAGES IS SUPERSEDED (2026-09-09).

Vitall's own cutter template **Capillary Test Kit Artwork for Window 169x122x23mm.pdf** arrived and is now in **assets/packaging/dieline/**. It disproves the fold assumption these pages are drawn to. The flat is **169 × 304 mm** with panels of **122 / 23 / 122 / 22**, so there is a **23 mm spine panel** and each face is **169 × 122 mm**, not the 179 × 152 mm halves drawn here. The front face is **30 mm too tall and 10 mm too wide** on every page below, and the layout needs re-drawing rather than scaling. **What IS current on these pages is the branding:** the Interlocked AP (no container) and the two-word ANDRO PRIME wordmark, both from the drawn vector masters, replaced the boxed monogram and the one-word wordmark on 2026-09-09.

Palette variant. #FFFFFF board, pure #000000 ink. Higher contrast and a colder, more clinical read; the compliance window becomes invisible until it is printed, since it is simply unprinted board. **The palette call is still open**, so this proof exists in both; geometry and copy are identical between them.

Route B from **concept-sleeve-fronts-v7-two-routes.html** transposed onto the real dimensions from Vitall's artwork file. Fronts are lifted verbatim from that concept, with one copy change. The back is new: Route B had fronts only, so it has been drawn in the same system and laid out around the compliance window.

THE ONE COPY CHANGE

"Thresholds signed off by Dr Ewa Lindo, GMC-registered GP" is removed from all three fronts. Removed programmatically and asserted at exactly three matches, so it cannot have been missed on one kit. **"ANALYSED IN A UKAS-ACCREDITED UK LABORATORY" stays.**

Worth a decision rather than an assumption: the Ewa attribution still appears on the live site and in approved copy. Taking it off the pack only is fine, but if the intent is that it is not needed anywhere, that is a decision sweep, not a packaging edit.

DIMENSIONS

Flat trim	179.00 × 304.00 mm → 169.00 × 304.00 mm per the cutter template. The 179 was the bleed box, not the trim (5 mm each side).
Folded face	179.00 × 152.00 mm → 169.00 × 122.00 mm . There is a separate 23 mm spine panel between the faces.
Fold	152.00 mm from trim top, assumed → panels 122 / 23 / 122 / 22 mm from the top, plus a ~15 mm glue tab, per the cutter template. The assumption was flagged honestly here and has now been disproved: there is a 23 mm spine panel , so the sleeve does not fold in half.
Bleed	3 mm all round → page is 185 × 310 mm
Die-cut aperture	DIE: 118.00 × 67.00 mm, corner radius r5.0 , from Vitall's cutter template. Our 108.00 × 57.00 is the same hole with the required 5 mm artwork bleed taken in, so both figures were right all along and the dispute is closed. corner radius — 3.2 mm → r5.0 confirmed. Back panel only (Keith, 2026-09-09): the front face carries no window.

WHAT THE APERTURE DOES TO ROUTE B

- **It does not touch the fronts.** Route B's marker table, headline and spine are all on the front face, which carries no window (confirmed below).
- **The back is banded around it:** brand and next step above, window clear, regulatory below. There is no room for anything else.
- **The spine flips to the right** on the back in reading orientation, so it wraps the same physical edge as the front's after the fold.
- **No QR on the sleeve.** Per the /activate deprecation the sampling QR belongs on the insert, and the kit is already linked at order creation

EMIPDORONY ANDRO PRIME

ANDRO PRIME



AT-HOME BLOOD TEST • TESTOSTERONE

Testosterone

Find out if testosterone is the cause.

TESTOSTERONE	NMOL/L
FREE TESTOSTERONE	PMOL/L
SHBG	NMOL/L
FREE ANDROGEN INDEX	INDEX
ALBUMIN	G/L

ANALYSED IN A UKAS-ACCREDITED UK LABORATORY

IVD

CE • UKCA

REF • AP-T01

ANDRO-PRIME.COM


FOLD (assumed) • 152.00

ANDRO-PRIME.COM

IVD

CE • UKCA

In-vitro diagnostic for self-collection. Read the enclosed instruction sheet before use.
Distributed by Andro Prime Ltd (Co. 17185839), UK.
Analysed in a UKAS-accredited UK Laboratory.
Store below 25°C. Do not use if the pouch is damaged.

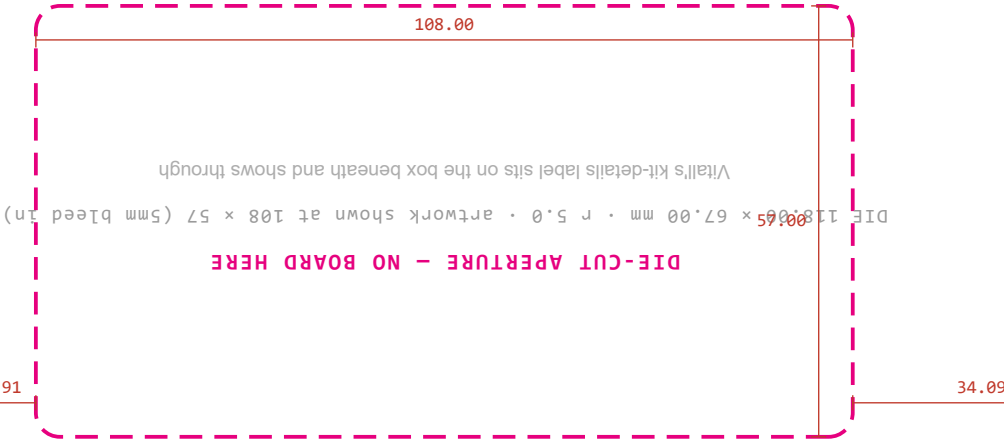

Read the enclosed instruction sheet before taking your sample.

SEE YOUR RESULTS AT ANDRO-PRIME.COM

Your kit is already linked to you. Nothing to register.

EMIPDORONA ANDRO PRIME

ANDRO PRIME



AT-HOME BLOOD TEST • ENERGY & RECOVERY

Energy & Recovery

Your levels, not your programme.

VITAMIN D	NMOL/L
ACTIVE B12	PMOL/L
HS-CRP	MG/L
FERRITIN	µG/L

ANALYSED IN A UKAS-ACCREDITED UK LABORATORY

IVD

CE • UKCA

REF • AP-E02

ANDRO-PRIME.COM

FOLD (assumed) • 152.00

ANDRO-PRIME.COM

CE • UKCA


IVD

In-vitro diagnostic for self-collection. Read the enclosed instruction sheet before use.

Distributed by Andro Prime Ltd (Co. 17185839), UK.

Analysed in a UKAS-accredited UK Laboratory.

Store below 25°C. Do not use if the pouch is damaged.

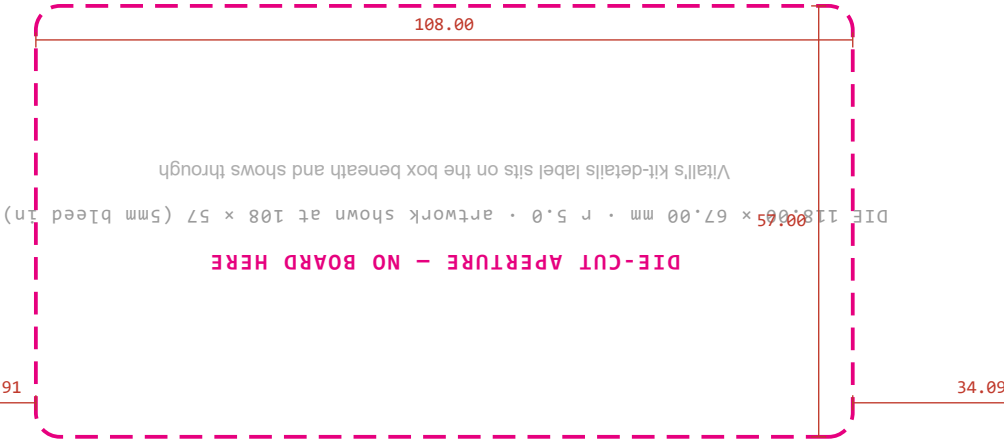

Read the enclosed instruction sheet before taking your sample.

SEE YOUR RESULTS AT ANDRO-PRIME.COM

Your kit is already linked to you. Nothing to register.



EMIPDORONY ANDRO PRIME

ANDRO PRIME



AT-HOME BLOOD TEST • NINE MARKERS

Hormone & Recovery

Nine markers. Hormones and recovery in one panel.

TESTOSTERONE	NMOL/L	VITAMIN D	NMOL/L
FREE TESTOSTERONE	PMOL/L	ACTIVE B12	PMOL/L
SHBG	NMOL/L	HS-CRP	MG/L
FREE ANDROGEN INDEX	INDEX	FERRITIN	µG/L
ALBUMIN	G/L		

ANALYSED IN A UKAS-ACCREDITED UK LABORATORY

IVD

CE • UKCA

REF • AP-H03

ANDRO-PRIME.COM


FOLD (assumed) • 152.00

ANDRO-PRIME.COM

CE • UKCA

IVD

In-vitro diagnostic for self-collection. Read the enclosed instruction sheet before use.
Distributed by Andro Prime Ltd (Co. 17185839), UK.
Analysed in a UKAS-accredited UK Laboratory.
Store below 25°C. Do not use if the pouch is damaged.

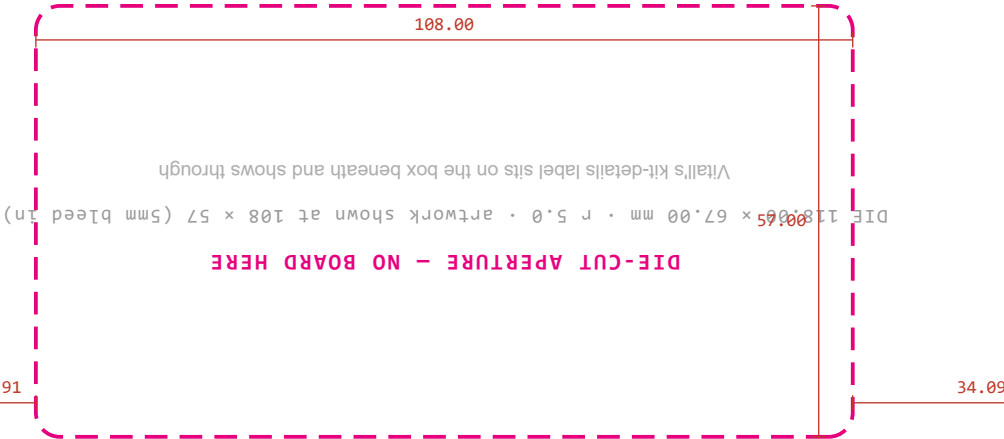

Read the enclosed instruction sheet before taking your sample.

SEE YOUR RESULTS AT ANDRO-PRIME.COM
Your kit is already linked to you. Nothing to register.




Sleeve back — reading orientation

UNIVERSAL ACROSS ALL THREE KITS · GEOMETRY SUPERSEDED 2026-09-09 · DO NOT PRINT



SEE YOUR RESULTS AT **ANDRO-PRIME.COM**
Your kit is already linked to you. Nothing to register.

Read the enclosed instruction sheet before taking your sample.

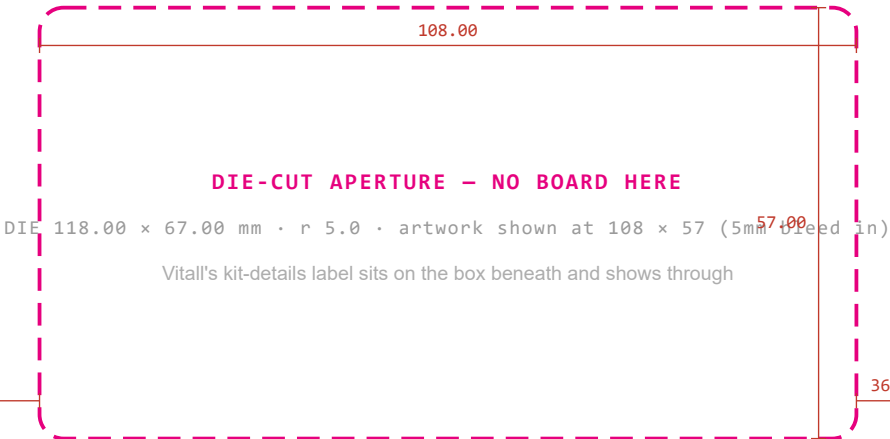


In-vitro diagnostic for self-collection. Read the enclosed instruction sheet before use.

Distributed by Andro Prime Ltd (Co. 17185839), UK.
Analysed in a UKAS-accredited UK laboratory.
Store below 25°C. Do not use if the pouch is damaged.

IVD CE · UKCA

ANDRO-PRIME.COM

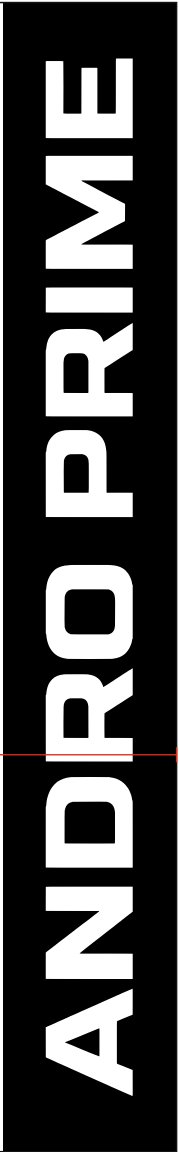

Band layout, forced by the aperture

- Above 0 – 47.50 mm brand + what to do next
- Cut 47.50 – 104.50 mm board REMOVED; Vitall's label on the box shows through
- Below 104.50 – 152.00 mm regulatory fine print

Why the black spine is on the right here

The fold preserves left-to-right, and the back is seen from the other side, so a spine drawn on the right in reading orientation wraps the same physical edge as the front's.