





Laparoscopy





GI endoscopy

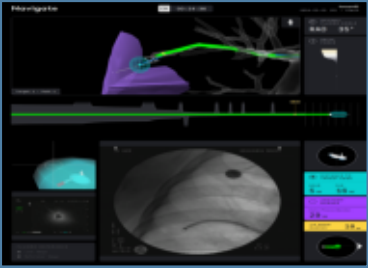


Bronchoscopy

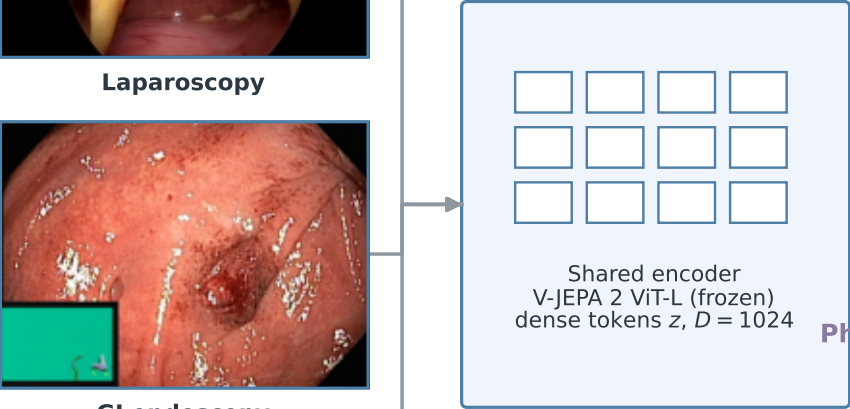

Passive-video forecast (validated)

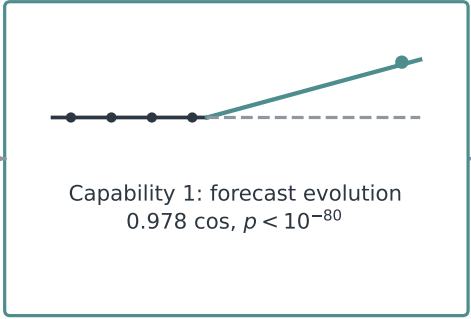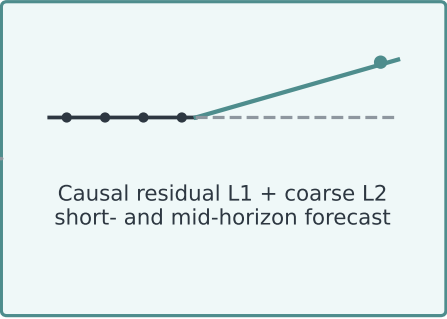



Clinical application pathways

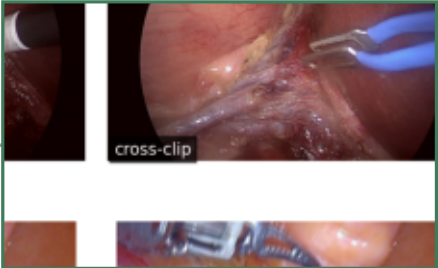

Forecast retrieval





Action-conditioned

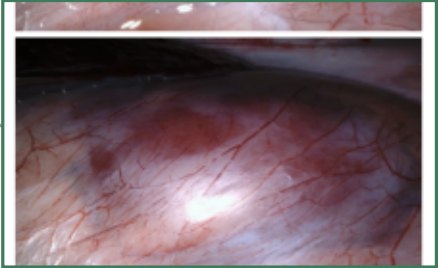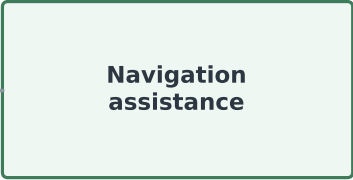

Navigation rollout

Physical grounding (audited; pose/depth-gated)

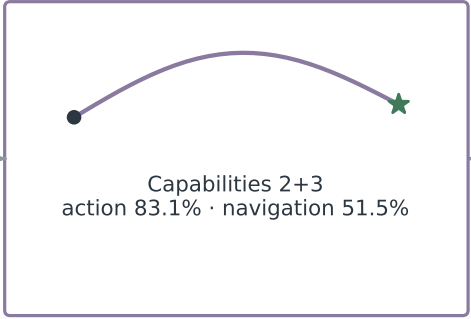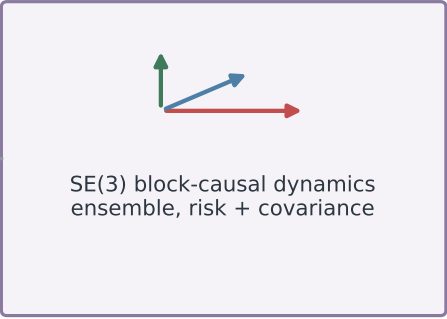

Input-sensitivity tests

history / action / domain

Reprojection pose gate

10.2 px -> 0.21 px

Matched negative banks

fixed, same-sequence

Grouped CV + frozen test

no test-set tuning