



Oscilloscope

Probe Calibration

Technician: Test

Test Date: 2026-01-03 12:41:06

Equipment: Test

Equipment ID: Test

Test Procedure: Test-1

Project: Test

Customer: Test

Temperature: 23

Humidity: 45


Location: Lab1

Overall Result: INCONCLUSIVE

Waveform Captures

Captured waveforms and analysis.

Waveforms

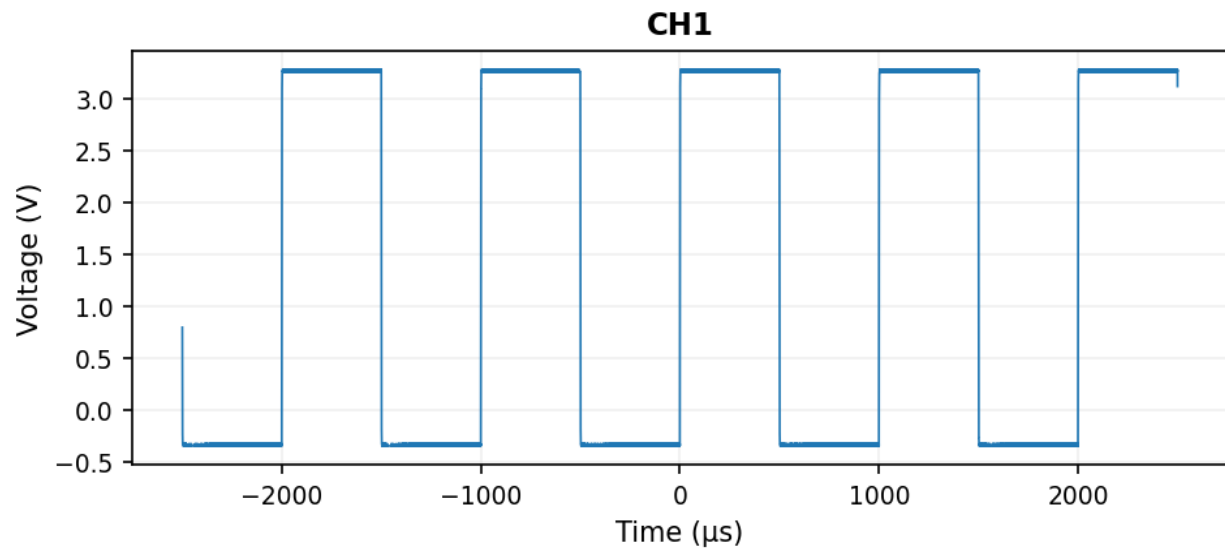

Channel: CH1
Sample Rate: 20.00 MS/s
Record Length: 100000 samples
Peak-to-Peak: 3.6200 V
Min: -0.3400 V
Max: 3.2800 V