



(a) Exact dose calibration
Graph coloring, 0.5B — one seed

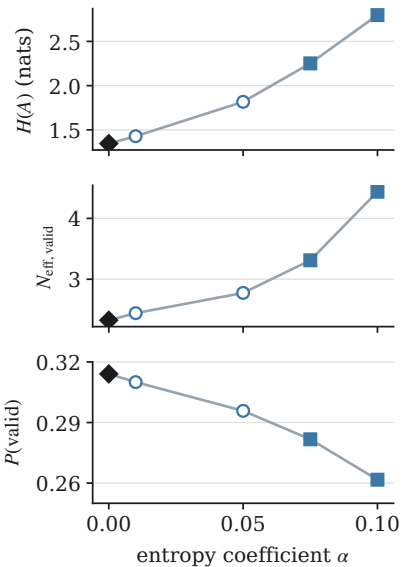

(b) 0.5B dynamics — exact training-prompt sensor (not held-out)

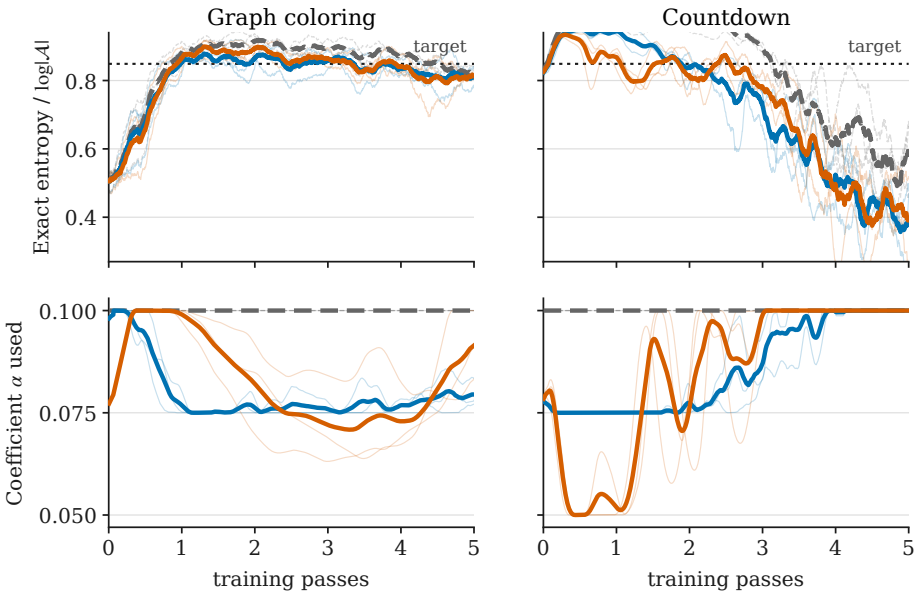

Controller curves: centered 0.125-pass mean; thin lines are seeds 43–45, heavy lines are their mean.