


## FS mirror, (dia25,4x6)mm, HR>99%@280-400, i0-45

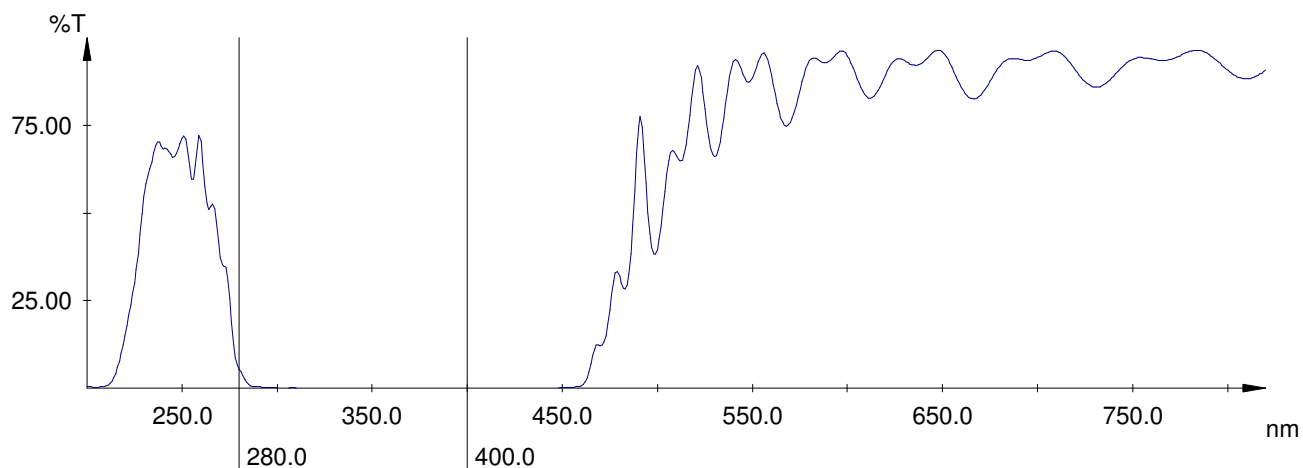

Title:  
Operator:  
List created on: 6/9/2021

<b>Designation</b>	<b>SPECORD 250 PLUS - 223G1076</b>
Date/Time	09/06/2021 08:50
Display	Transmittance
Correction	Reference
Slit	4 nm
Lamp change at	320 nm
no pre-monochromator from	190 nm

<b>Meas. mode</b>	<b>Spectral Scan</b>
Range [nm]	200 - 820
Delta lambda [nm]	1
Speed [nm/s]	2

### Measured values

280.0 nm	%T
Sample 1	5.32

400.0 nm	%T
Sample 1	0.02