
Autotune - 5977

Tune timestamp: 9/22/2026 1:26 PM (UTC+09:00) GCMSD

D:\MASSHUNTER\GCMS\1\5977\atune.u US1426M313

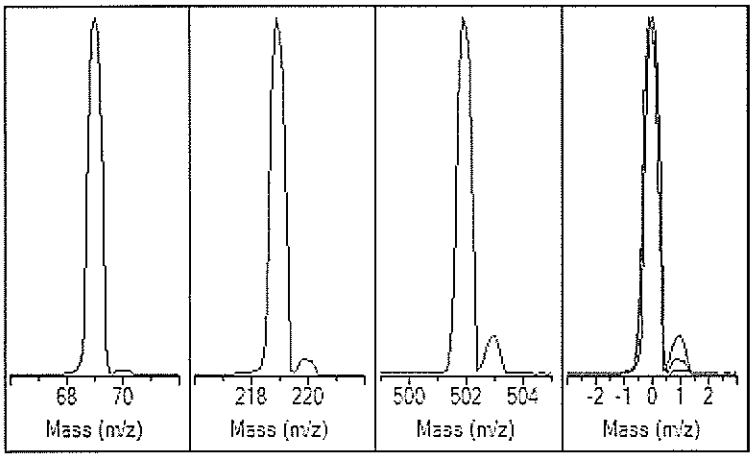


Ion Polarity	Pos	PFTBA	Open
Emission	34.6	Mass Gain	-753
Electron Energy	70.0	Mass Offset	-34
Filament	2	Amu Gain	833
Repeller	34.90	Amu Offset	124.75
Ion Focus	79.5	Width219	-0.012
Entrance Lens	7.5	DC Polarity	Pos
Ent Lens Offset	17.18	HED Enable	On
Ion Body	0.00	EM Volts	1477.8
Post Extractor 1	0	Extractor Lens	0.00
Post Extractor 2	0	Scan Speed	3
JetClean Flow	0	Averages	3

Actual m/z	Abund	Rel Abund	Pw50
69.00	373,181	100.0%	0.60
218.90	306,393	82.1%	0.60
501.90	19,275	5.2%	0.60

Temperatures and Pressures

MS Source	230	Turbo Speed	100.0
MS Quad	150	Hi Vac	8.52e-06

Low	High	Step	Speed	Threshold	Peaks	Base	Abundance	Total Ion
10.00	701.00	0.10	3	100	98	69.00	362,304	1,199,833

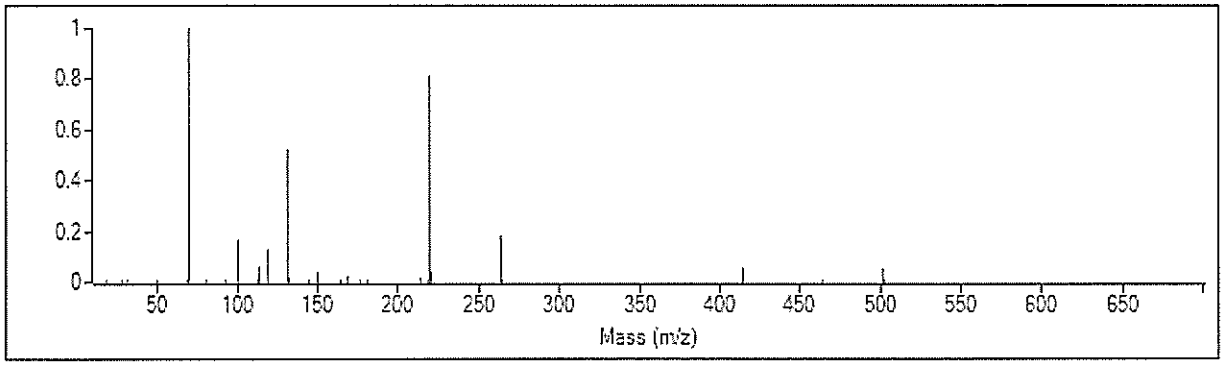

Target m/z	Actual m/z	Abund	Rel Abund	Iso m/z	Iso Abund	Iso Ratio
69.00	69.00	362,304	100.0%	70.00	4,043	1.1%
219.00	219.00	292,864	80.8%	220.00	12,654	4.3%
502.00	502.00	18,800	5.2%	503.00	1,818	9.7%

Air/Water Check: H20 ~0.4% N2 ~0.7% O2 ~0.2% CO2 ~0.0% N2/H20 ~182.0%

Column(1) Flow: 1.00 Column(2): 0.00 ml/min Interface Temp: 280

Ramp Criteria:

Ion Focus maximum 90 volts using ion 502; Electron Multiplier Gain 29800.767

Repeller maximum 35 volts using ion 219; Gain Factor 0.2980

Mass Gain Values(Scan Speed): -742(3) -736(2) -721(1) -705(0) -652(FS1) -635(FS2)

TARGET MASS:	50	69	131	219	414	502	1050
Amu Offset	124.8	124.8	124.8	124.8	124.8	124.8	124.8
Entrance Lens Offset	17.2	17.2	17.2	17.2	17.2	17.2	17.2