TEST REPORT

E: contact@tjqxgd.com
W: www.tjqxgd.com


TSM5-20260908S6179 **Sample Received: 2026-09-08**

Authentication Code: **Analysis date: 2026-09-09**




Compound	TSM5/Tesamorelin	CAS Number	218949-48-5
Formula	$C_{221}H_{366}N_{72}O_{67}S$	Molecular Weight	5136.0
Batch Number	5828704		
Manufacturer	https://pllaboratory.com Telegram:@Factory_Global		

HPLC-MS Details:

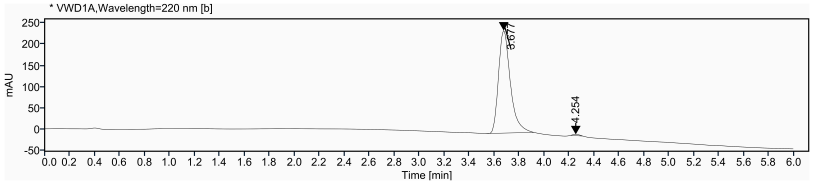

Signal: * VWD1A,Wavelength=220 nm [b]

RT [min]	Type	Width [min]	Area	Height	Area%
3.677	MM m	0.3881	1591.7281	241.7475	99.3011
4.254	MM m	0.0993	11.2022	3.0263	0.6989
		Sum	**1602.9303**		

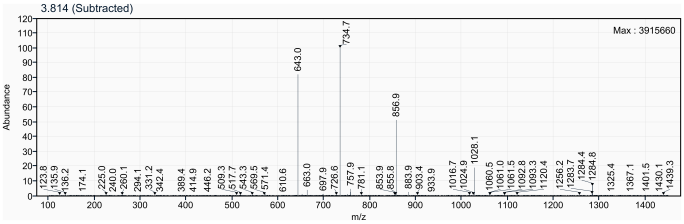

Result:

Test Items	Specification	Results
Appearance	White to off-white powder	White powder
Purity (LCMS/HPLC)	≥ 99.0%	99.30%
Mass Spectrum	Conforms to $[M+8/7/6/5/4H]^{8/7/6/5/4+}$	Detected
Peptide Weight	4.83 mg	

Peng Gao, Data Compilation Zhibo Li, Technical Review


重要声明 / Important Notice


本检测数据由第三方合作实验室提供，本公司负责数据整理、审核与文件出具。本公司及合作检测方均不持有 CMA/CNAS 认证资质，本文件不具有法定证明效力，不得用于监管申报、诉讼举证或其他要求法定认证文件的用途。相关产品仅限科学研究用途，不得用于人类或兽医用途、诊断、治疗或临床应用。


This test data is provided by a third-party partner laboratory; our company is responsible for data compilation, review, and issuance of the document. Neither our company nor the partner testing laboratory holds CMA/CNAS accreditation, and this document does not carry legal certification validity. It shall not be used for regulatory submissions, litigation evidence, or any other purpose requiring legally accredited documentation. The related products are intended for scientific research use only and have not been approved for human or veterinary use, diagnosis, treatment, or clinical application. Results should be interpreted by qualified professionals within the intended scope of research.


LCMS Sample Purity - Detailed Report

Result set name:	SingleSample		
Data file:	TSM5.dx	**Project name:**	2026
Sample name:	TSM5	**Operator:**	admin
Instrument:	LCMS	**Acquired on:**	2026-09-09 10:04:03+08:00
Inj. volume:	5.000 µL	**Location:**	P1-E1
Acq. method:	LCMS-02AB.amx		
Processing method:	LCMS-LJJ.pmx		

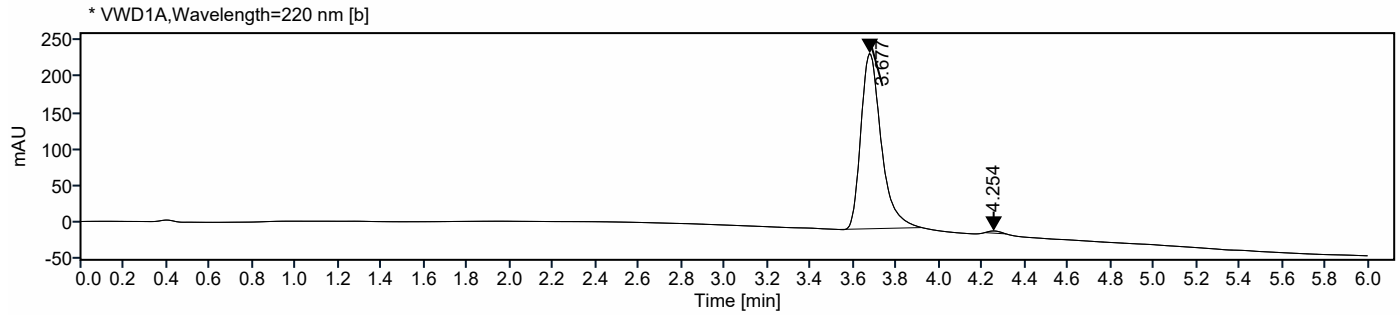

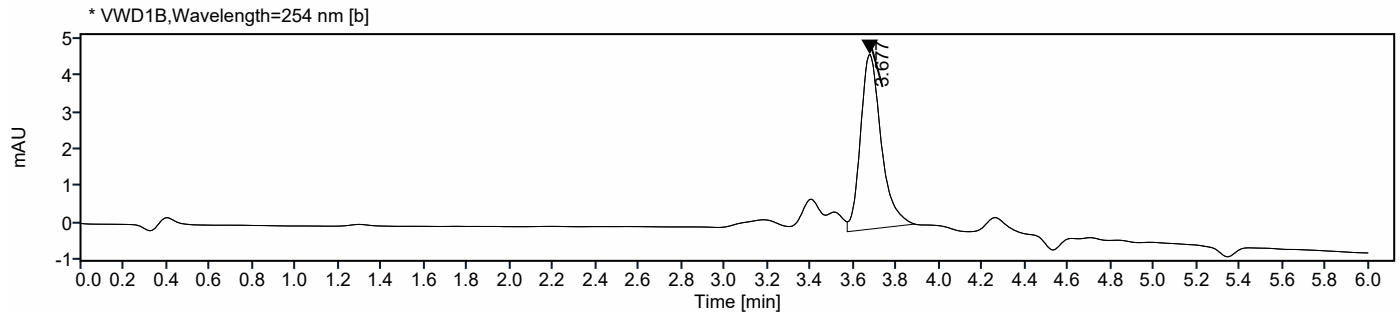

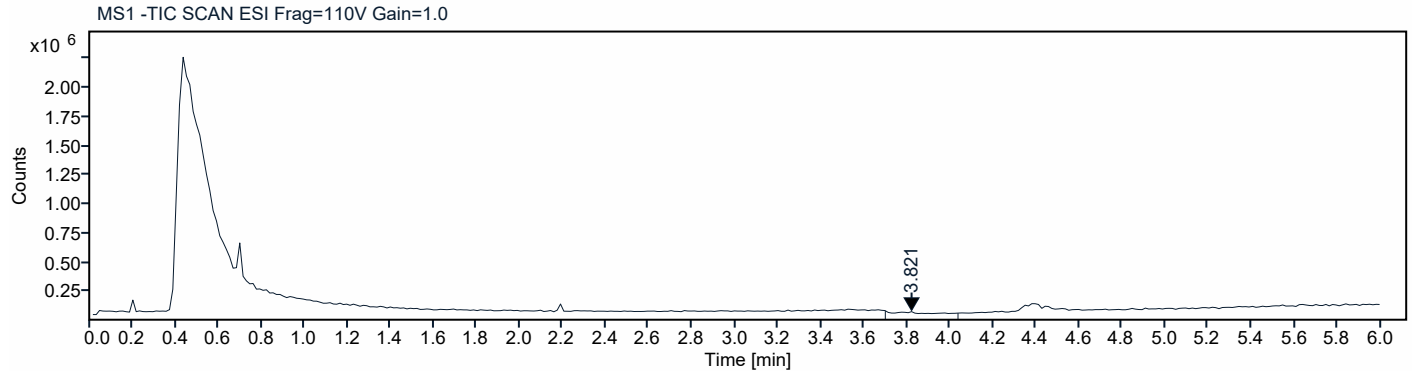

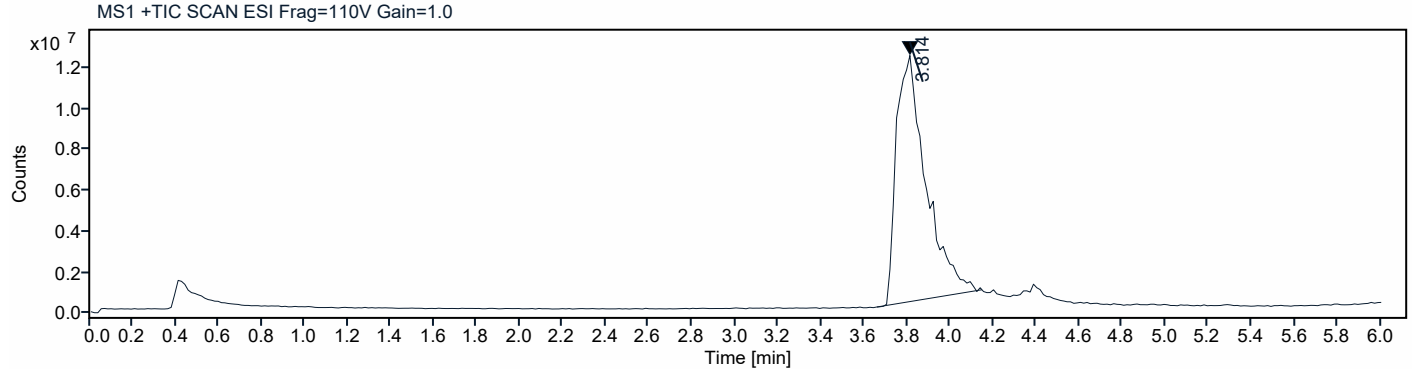

Signal: MS1 +TIC SCAN ESI Frag=110V Gain=1.0

RT [min]	Type	Width [min]	Area	Height	Area%
3.814	MM m	0.4876	114791577.7869	11992446.8578	100.0000
		Sum	**114791577.7869**		

Signal: MS1 -TIC SCAN ESI Frag=110V Gain=1.0

RT [min]	Type	Width [min]	Area	Height	Area%
3.821	MM m	0.3377	3431193.6081	175174.6357	100.0000
		Sum	**3431193.6081**		

Signal: * VWD1A,Wavelength=220 nm [b]

RT [min]	Type	Width [min]	Area	Height	Area%
3.677	MM m	0.3881	1591.7281	241.7475	99.3011
4.254	MM m	0.0993	11.2022	3.0263	0.6989
		Sum	**1602.9303**		


Signal: * VWD1B,Wavelength=254 nm [b]

RT [min]	Type	Width [min]	Area	Height	Area%
3.677	VM m	0.3147	31.7298	4.7455	100.0000
		Sum	**31.7298**		

Peak Details (Area Percent at least 1%)

Signal Description: MS1 +TIC SCAN ESI Frag=110V Gain=1.0

Peak RT: 3.814 min **Area %:** 100.00%

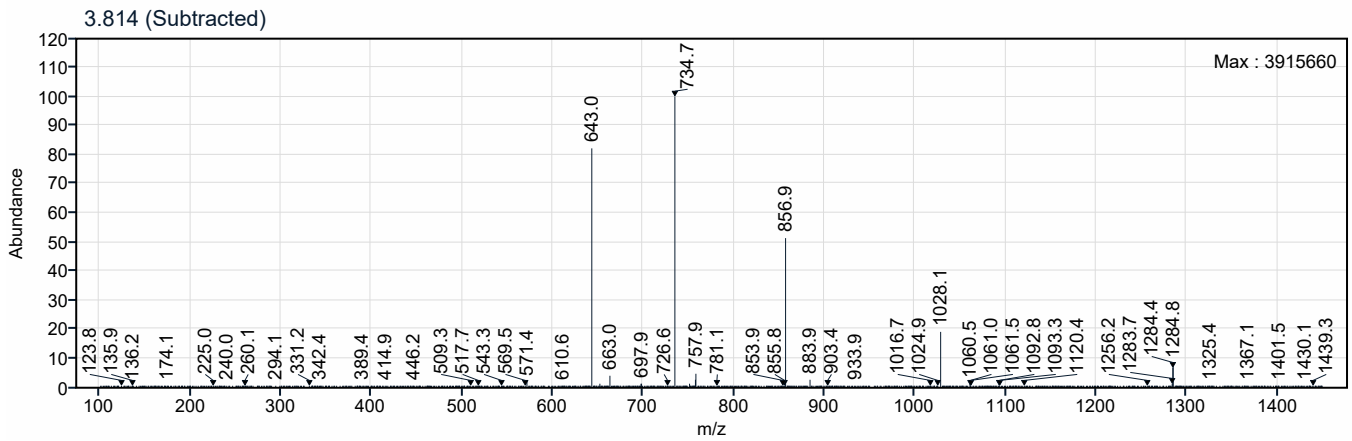

Signal Description: MS1 -TIC SCAN ESI Frag=110V Gain=1.0

Peak RT: 3.821 min **Area %:** 100.00%

