



Case number CAS-0022102876

Order number WO-31212303 | Visit Date 01/16/2025

Instrument Details		Customer Details	
Instrument/Module	cobas 6800	Customer Number	0052027574
Serial Number	1376	Customer Name	P'CHOMKLAO HOSPITAL รพ.พระจอมเกล้า
Internal Instrument Name		Street Address	53 ถ.รถไฟ ต.คลองกระเซง
		ZIP	76000 - Phetchaburi
		Contact Name	Supaporn Sae-aeaw
		Contact Phone	+66864684997
Additional Details			
	PO		

Service Activity Code Service Visit

Purpose of Visit

Instrument: cobas 6800 (S/N 1376), P'CHOMKLAO HOSPITAL รพ.พระจอมเกล้า

Issue: The instrument could not be completely initialized after performing periodic maintenance. Prolonged initializing status was observed after performing periodic maintenance.

Action: The customer restarted the instrument. The instrument could then be completely initialized and was back to standby status.

Solution was communicated to the customer on 08 Jan 2024

Inform territory FSE for more inspection and monitoring of the issue.

Performed Activities

- Replace Control unit reagent storage
- Reagent Storage drawer adjustment
- Consumable loading area teach
- Reagent Storage check


Time Report

Category	Start	End	Hours	Billing Type
05913616001-Service labour time	01/16/2025 9:01 AM	01/16/2025 5:00 PM	7.98	Free of Charge

Signature or Stamp

Customer Supaporn Sae-aeaw	Roche Support Sompop Bangyeekhan
-------------------------------	-------------------------------------

Sign here

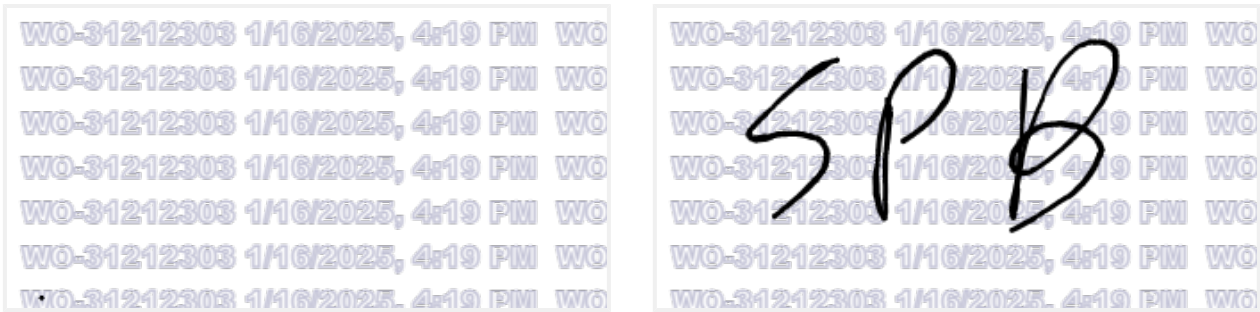

By signing this document

- Customer representative confirms they have reviewed the work carried out as described and accepts the system for use.
- Roche Support person confirms the above mentioned work and checks have been completed..
- .