



Case number CAS-0023895830

Order number WO-33719531 | Visit Date 08/17/2025

Instrument Details

Instrument/Module cobas 6800

Serial Number 1376

Internal Instrument Name

Additional Details

PO

Customer Details

Customer Number 0052027574

Customer Name P'CHOMKLAO HOSPITAL
รพ.พระจอมเกล้า

Street Address 53 ถ.รถไฟ ต.คลองกระเซง

ZIP 76000 - Phetchaburi

Contact Name Supaporn Sae-aeaw

Contact Phone +66864684997

Service Activity Code Service Visit

Purpose of Visit

Instrument: S/N 1376 - cobas 6800

Location: P'CHOMKLAO HOSPITAL รพ.พระจอมเกล้า

Issue: Maintenance action failed. - Backup failed

Backup, details: Files created locally, because the backup settings are unavailable.

Permission denied. (6284.1.01.01.07)

Action:

- Remote UI was already turned on
- Test connection: connectivity okay
- Stopped freeSFTPdservices

But the maintenance still failed.

Solution: FSE (K.Sompop) will investigate on this case.

Performed Activities

- Check Physical Connection
- Check Computer D drive is Full
- Check SW FreeFTP root directory are wrong
- Reconfig root diretory and delete old data
- Back up and Archive are passed
- Re-connect Touch Screen cable

Time Report



Category	Start	End	Hours	Billing Type
05913616001-Service labour time	08/17/2025 9:01 AM	08/17/2025 12:00 PM	2.98	Free of Charge

Signature or Stamp

Customer
Supaporn Sae-aeaw

Roche Support
Sompop Bangyeekhan

Sign here

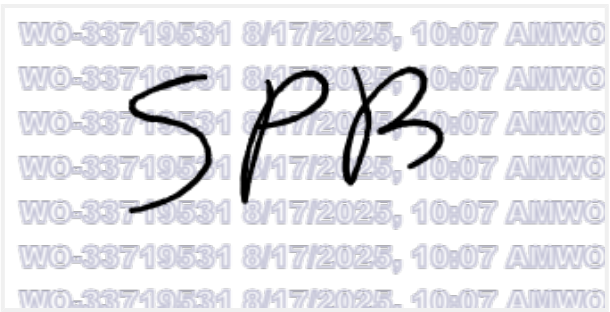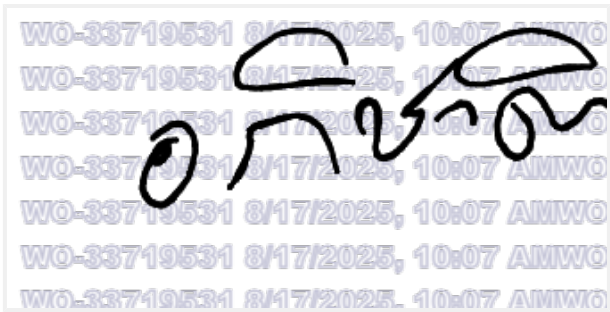

By signing this document

- Customer representative confirms they have reviewed the work carried out as described and accepts the system for use.
- Roche Support person confirms the above mentioned work and checks have been completed..
- .

Hotline : 1800-0193-99
Tel : 02 7912200
Line Id : @rcscthailand

Roche Customer Support Center