



Case number CAS-0022679352

Order number WO-31932300 | Visit Date 03/21/2025

| Instrument Details       |            | Customer Details |                                       |
|--------------------------|------------|------------------|---------------------------------------|
| Instrument/Module        | cobas 6800 | Customer Number  | 0052027574                            |
| Serial Number            | 1376       | Customer Name    | P'CHOMKLAO HOSPITAL<br>รพ.พระจอมเกล้า |
| Internal Instrument Name |            | Street Address   | 53 ถ.รถไฟ ต.คลองกระเซง                |
|                          |            | ZIP              | 76000 - Phetchaburi                   |
|                          |            | Contact Name     | Supaporn Sae-aeaw                     |
|                          |            | Contact Phone    | +66864684997                          |
| Additional Details       |            |                  |                                       |
|                          | PO         |                  |                                       |

Service Activity Code Service Visit

Purpose of Visit

Issue: The customer has alleged that cobas 6800 (S/N 1376) transfer module changed to error after loading the sample racks to the instrument. Sample transport unit hook motor: Movement error occurred. Possible cause: a position deviation error occurred.

Action:

- Suggested that the customer rechecked the sample rack in the transfer module and found that one rack was stuck because the sample transport unit hook jammed.
- Restarted the system from error status but the instrument was still error.
- Informed territory FSE for further investigation and onsite repair visit.

Performed Activities

- Recheck connection ssm and transfer module
- Restart full system c6800 and ssm
- Test feedrack (pass)

Time Report


| Category                        | Start              | End                | Hours | Billing Type   |
|---------------------------------|--------------------|--------------------|-------|----------------|
| 05913616001-Service labour time | 03/21/2025 2:31 PM | 03/21/2025 5:01 PM | 2.50  | Free of Charge |

Signature or Stamp

Customer  
Supaporn Sae-aeaw

Roche Support  
Chanon Ittisakulphun

Sign here

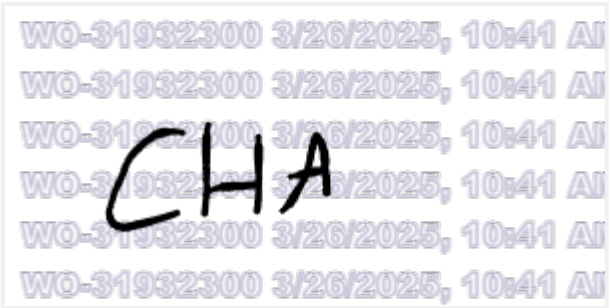

By signing this document  
- Customer representative confirms they have reviewed the work carried out as described and accepts the system for use.  
- Roche Support person confirms the above mentioned work and checks have been completed..  
- .

Hotline : 1800-0193-99  
Tel : 02 7912200  
Line Id : @rcscthailand

Roche Customer Support Center