



Case number CAS-0025277462

Order number WO-35702613 | Visit Date 02/25/2026

Instrument Details

Instrument/Module cobas 6800

Serial Number 1376

Internal Instrument Name

Additional Details

PO

Customer Details

Customer Number 0052027574

Customer Name P'CHOMKLAO HOSPITAL
รพ.พระจอมเกล้า

Street Address 53 ถ.รถไฟ ต.คลองกระเซง

ZIP 76000 - Phetchaburi

Contact Name Supaporn Sae-aeaw

Contact Phone +66864684997

Service Activity Code Service Visit

Purpose of Visit

Instrument: cobas 6800 V2 (S/N 1376), P'CHOMKLAO HOSPITAL

Issue: Transfer module error occurred during HIV-1 sample transfer (73 samples + 3 controls). No reagent was lost.

Action:

- Advised the customer to perform transfer module cleanup and then it returned to standby .
- The customer confirmed that the sample transfer head teaching and the tightness check were done before running.
- Upon analyzing the PR by Tellme, no additional data was obtained. However, the similar issue was previously found on 11 Feb 2026.
- Transferred the case to FSE (K. Chanon) for further inspection.

Performed Activities

- Replace Sample transfer head (D)
- Sample transfer head teach,tightness check,tip handling check (pass)
- Run sample (pass)

Time Report


Category	Start	End	Hours	Billing Type
05913616001-Service labour time	02/25/2026 11:00 AM	02/25/2026 3:00 PM	4	Free of Charge

Signature or Stamp

Customer
Supaporn Sae-aeaw

Roche Support
Chanon Ittisakulphun

Sign here

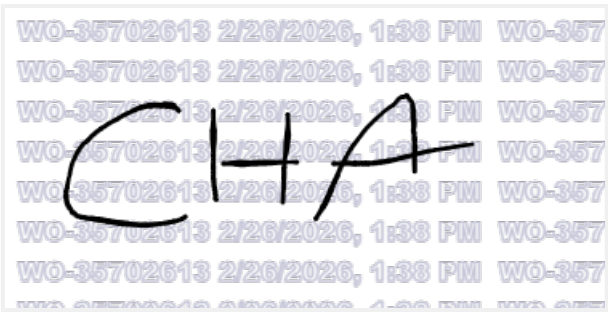

By signing this document
- Customer representative confirms they have reviewed the work carried out as described and accepts the system for use.
- Roche Support person confirms the above mentioned work and checks have been completed..
- .

Hotline : 1800-0193-99
Tel : 02 7912200
Line Id : @rcscthailand

Roche Customer Support Center