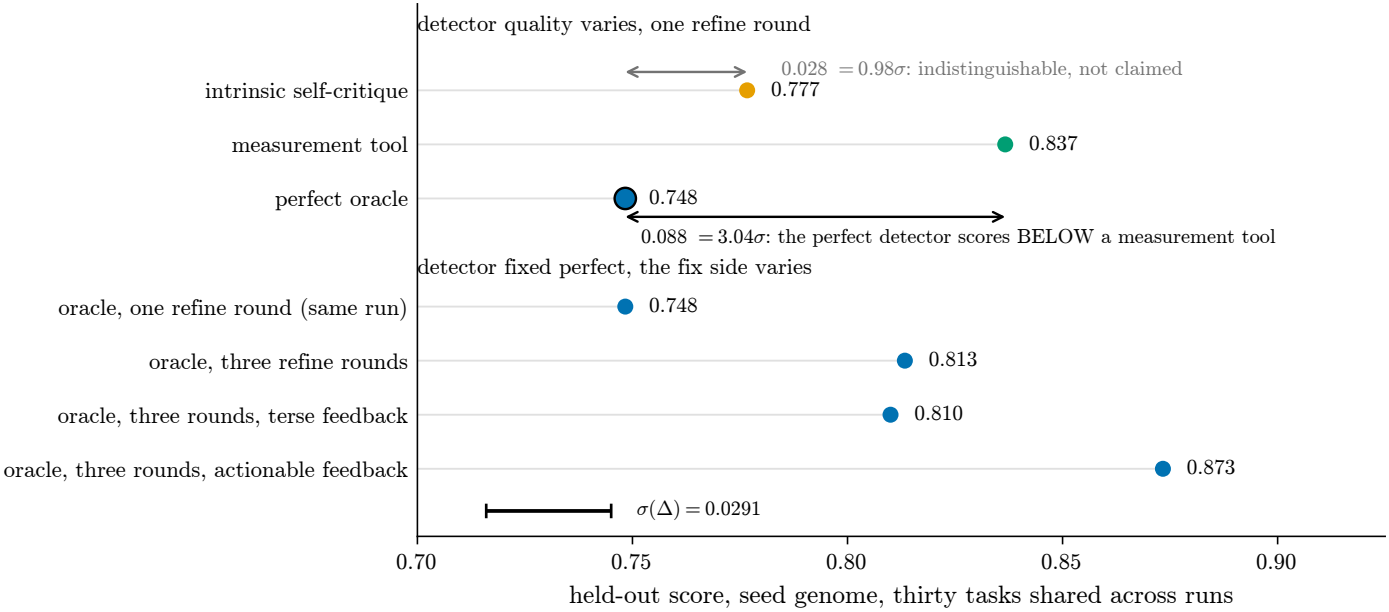
detector quality varies, one refine round
0.028 = 0.98σ: indistinguishable, not claimed
intrinsic self-critique
0.777
measurement tool
0.837
perfect oracle
0.748
0.088 = 3.04σ: the perfect detector scores BELOW a measurement tool
detector fixed perfect, the fix side varies
oracle, one refine round (same run)
0.748
oracle, three refine rounds
0.813
oracle, three rounds, terse feedback
0.810
oracle, three rounds, actionable feedback
0.873
σ(Δ) = 0.0291
0.70
0.75
0.80
0.85
0.90
held-out score, seed genome, thirty tasks shared across runs