



## DS-7000 Series with HLX-561 Telemetry Transmitter

DS-7000 Series Central Monitor

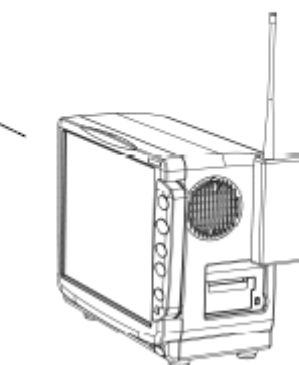

DS-7000 Bedside Monitor

### [Rear Side]

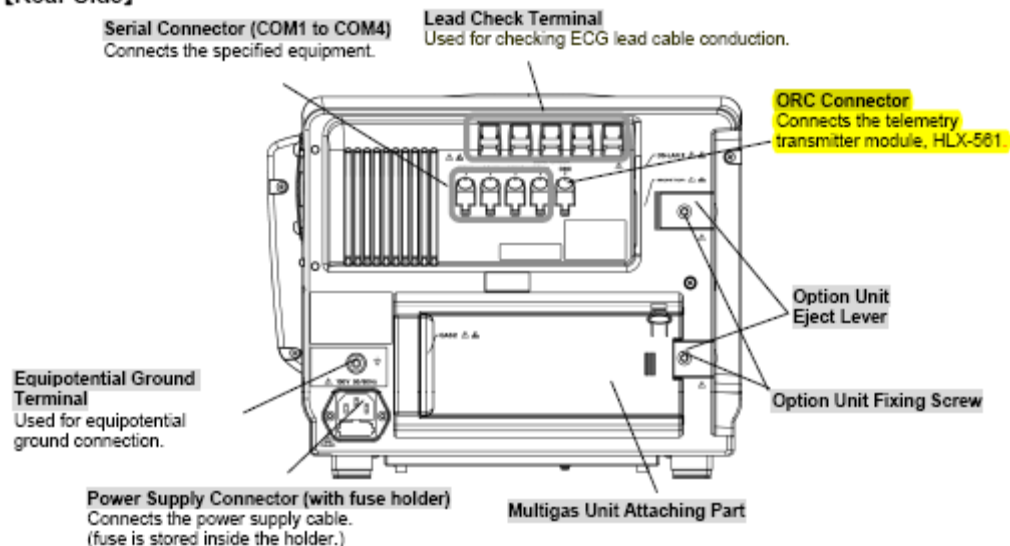

### Requires the following parts for Telemetry Operation

- HLX-561 - Multiparameter Telemetry Transmitter.
- OAO-23A - Wire Adapter (NOT IN STOCK)

### Only the following Waveforms can be transmitted.

ECG1 / RESP / CO2 / BP1 / BP2 / SPO2

\* RESP will not be transmitted if APNEA source is CO2.

or

ECG1 / ECG2 / RESP / CO2 / BP1 / SPO2

\* Either CO2 and RESP will be transmitted based on Apnea source.