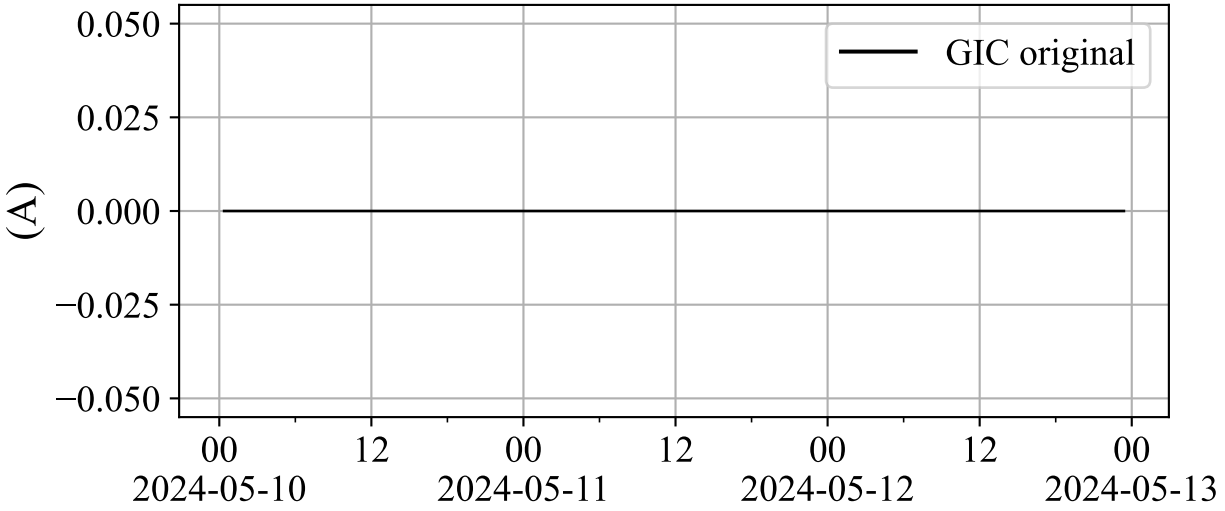Manual Error: stays at zero
Automated Error: All GIC values are positive;
All GIC values are negative;
Low signal: all GIC values within +/- 4 A;
Cadence is >= 60 seconds (3600.0 seconds);
Data gap detected >= 10.0 minutes (3600.0 seconds);
Data gap detected >= 10.0 minutes (3600 seconds) due to NaN values;
Data is constant for at least 5 minutes starting at time 2024-05-10 15:22:46