Technical manual contents

Procedure 1 — label M-2; physical 2

Procedure 2 — label M-6; physical 6

Procedure 1

Contents physical 1 ; final procedure label M-6 ; final physical 6.

One logical procedure keeps its numbered instruction and rich children together in reading order.

100. Prepare procedure 1 without losing source whitespace.

```
verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1

verify = procedure_1
```

Procedure 1 running

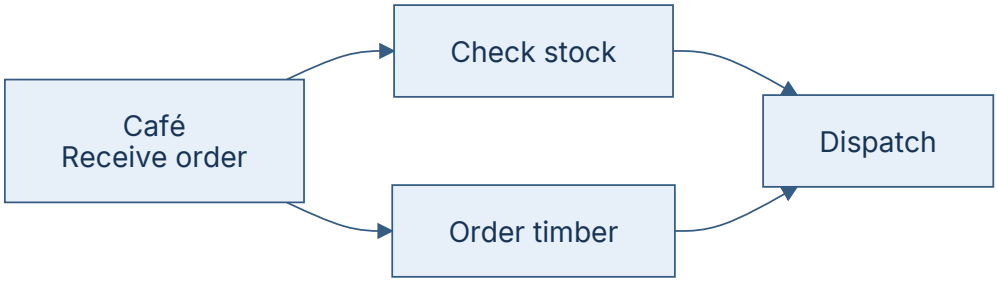

Prepared procedure diagram 1

The continued table remains inside the instruction and both callout panels.

Procedure 1 checklist

Step	Contents label M-1
Step 1	Retain the procedure, its boxed instructions and the measured table columns.
Step 2	Retain the procedure, its boxed instructions and the measured table columns.
Step 3	Retain the procedure, its boxed instructions and the measured table columns.
Step 4	Retain the procedure, its boxed instructions and the measured table columns.
Step 5	Retain the procedure, its boxed instructions and the measured table columns.
Step 6	Retain the procedure, its boxed instructions and the measured table columns.
Step 7	Retain the procedure, its boxed instructions and the measured table columns.
Step 8	Retain the procedure, its boxed instructions and the measured table columns.
Step 9	Retain the procedure, its boxed instructions and the measured table columns.
Step 10	Retain the procedure, its boxed instructions and the measured table columns.
Step 11	Retain the procedure, its boxed instructions and the measured table columns.
Step 12	Retain the procedure, its boxed instructions and the measured table columns.

Procedure 1 running

Step	Contents label M-1
Step 13	Retain the procedure, its boxed instructions and the measured table columns.
Step 14	Retain the procedure, its boxed instructions and the measured table columns.
Step 15	Retain the procedure, its boxed instructions and the measured table columns.
Step 16	Retain the procedure, its boxed instructions and the measured table columns.
Step 17	Retain the procedure, its boxed instructions and the measured table columns.
Step 18	Retain the procedure, its boxed instructions and the measured table columns.
Step 19	Retain the procedure, its boxed instructions and the measured table columns.
Step 20	Retain the procedure, its boxed instructions and the measured table columns.
Step 21	Retain the procedure, its boxed instructions and the measured table columns.
Step 22	Retain the procedure, its boxed instructions and the measured table columns.
Step 23	Retain the procedure, its boxed instructions and the measured table columns.
Step 24	Retain the procedure, its boxed instructions and the measured table columns.
Step 25	Retain the procedure, its boxed instructions and the measured table columns.
Step 26	Retain the procedure, its boxed instructions and the measured table columns.
Step 27	Retain the procedure, its boxed instructions and the measured table columns.
Step 28	Retain the procedure, its boxed instructions and the measured table columns.
Step 29	Retain the procedure, its boxed instructions and the measured table columns.
Step 30	Retain the procedure, its boxed instructions and the measured table columns.

Procedure 1 running

Step	Contents label M-1
Step 31	Retain the procedure, its boxed instructions and the measured table columns.
Step 32	Retain the procedure, its boxed instructions and the measured table columns.
Step 33	Retain the procedure, its boxed instructions and the measured table columns.
Step 34	Retain the procedure, its boxed instructions and the measured table columns.
Step 35	Retain the procedure, its boxed instructions and the measured table columns.
Step 36	Retain the procedure, its boxed instructions and the measured table columns.
Step 37	Retain the procedure, its boxed instructions and the measured table columns.
Step 38	Retain the procedure, its boxed instructions and the measured table columns.
Step 39	Retain the procedure, its boxed instructions and the measured table columns.
Step 40	Retain the procedure, its boxed instructions and the measured table columns.

The inner callout closes after the complete checklist.

Complete procedure 1 before the next chapter begins.

The outer callout closes after its one logical instruction.

Procedure 2

Contents physical 1 ; final procedure label M-6 ; final physical 6.

One logical procedure keeps its numbered instruction and rich children together in reading order.

100. Prepare procedure 2 without losing source whitespace.

```
verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2

verify = procedure_2
```

Procedure 2 running

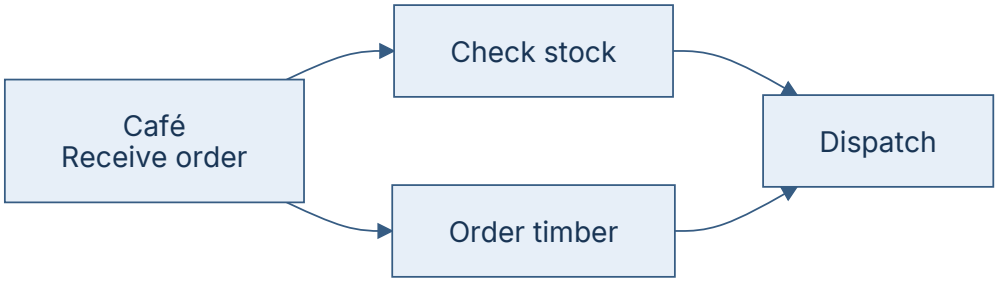

Prepared procedure diagram 2

The continued table remains inside the instruction and both callout panels.

Procedure 2 checklist

Step	Contents label M-1
Step 1	Retain the procedure, its boxed instructions and the measured table columns.
Step 2	Retain the procedure, its boxed instructions and the measured table columns.
Step 3	Retain the procedure, its boxed instructions and the measured table columns.
Step 4	Retain the procedure, its boxed instructions and the measured table columns.
Step 5	Retain the procedure, its boxed instructions and the measured table columns.
Step 6	Retain the procedure, its boxed instructions and the measured table columns.
Step 7	Retain the procedure, its boxed instructions and the measured table columns.
Step 8	Retain the procedure, its boxed instructions and the measured table columns.
Step 9	Retain the procedure, its boxed instructions and the measured table columns.
Step 10	Retain the procedure, its boxed instructions and the measured table columns.
Step 11	Retain the procedure, its boxed instructions and the measured table columns.
Step 12	Retain the procedure, its boxed instructions and the measured table columns.

Procedure 2 running

Step	Contents label M-1
Step 13	Retain the procedure, its boxed instructions and the measured table columns.
Step 14	Retain the procedure, its boxed instructions and the measured table columns.
Step 15	Retain the procedure, its boxed instructions and the measured table columns.
Step 16	Retain the procedure, its boxed instructions and the measured table columns.
Step 17	Retain the procedure, its boxed instructions and the measured table columns.
Step 18	Retain the procedure, its boxed instructions and the measured table columns.
Step 19	Retain the procedure, its boxed instructions and the measured table columns.
Step 20	Retain the procedure, its boxed instructions and the measured table columns.
Step 21	Retain the procedure, its boxed instructions and the measured table columns.
Step 22	Retain the procedure, its boxed instructions and the measured table columns.
Step 23	Retain the procedure, its boxed instructions and the measured table columns.
Step 24	Retain the procedure, its boxed instructions and the measured table columns.
Step 25	Retain the procedure, its boxed instructions and the measured table columns.
Step 26	Retain the procedure, its boxed instructions and the measured table columns.
Step 27	Retain the procedure, its boxed instructions and the measured table columns.
Step 28	Retain the procedure, its boxed instructions and the measured table columns.
Step 29	Retain the procedure, its boxed instructions and the measured table columns.
Step 30	Retain the procedure, its boxed instructions and the measured table columns.

Procedure 2 running

Step	Contents label M-1
Step 31	Retain the procedure, its boxed instructions and the measured table columns.
Step 32	Retain the procedure, its boxed instructions and the measured table columns.
Step 33	Retain the procedure, its boxed instructions and the measured table columns.
Step 34	Retain the procedure, its boxed instructions and the measured table columns.
Step 35	Retain the procedure, its boxed instructions and the measured table columns.
Step 36	Retain the procedure, its boxed instructions and the measured table columns.
Step 37	Retain the procedure, its boxed instructions and the measured table columns.
Step 38	Retain the procedure, its boxed instructions and the measured table columns.
Step 39	Retain the procedure, its boxed instructions and the measured table columns.
Step 40	Retain the procedure, its boxed instructions and the measured table columns.

The inner callout closes after the complete checklist.

Complete procedure 2 before the next chapter begins.

The outer callout closes after its one logical instruction.