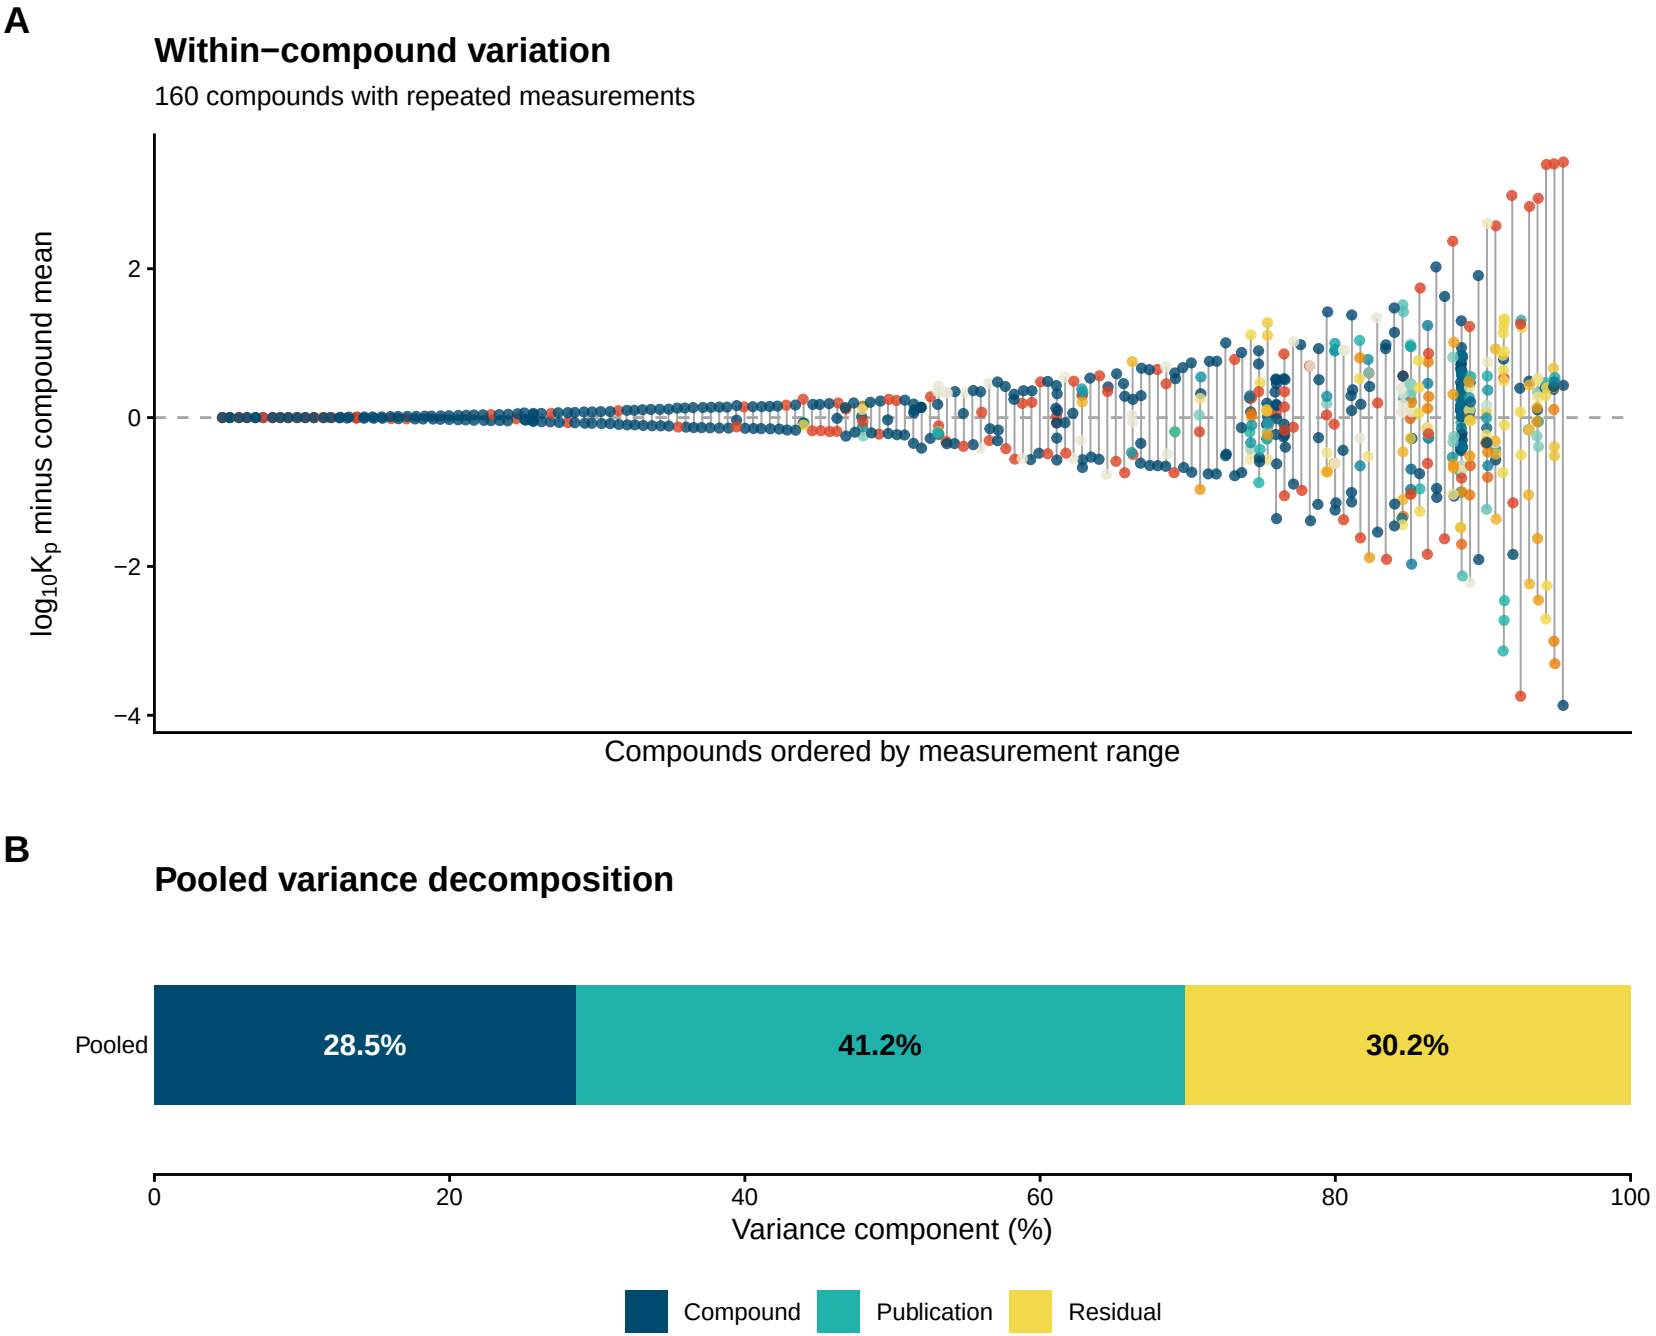
A
Within−compound variation
160 compounds with repeated measurements
log10Kp minus compound mean
2
0
−2
−4
Compounds ordered by measurement range
B
Pooled variance decomposition
Pooled
28.5%
41.2%
30.2%
0
20
40
60
80
100
Variance component (%)
Compound
Publication
Residual